Technical Information **Proline Promass H 500**

Coriolis flowmeter



The chemically resistant single-tube flowmeter, as remote version with up to 4 I/Os

Application

- Measuring principle operates independently of physical fluid properties such as viscosity or density
- Measuring highly accurately liquids and gases in applications requiring highest corrosion resistance

Device properties

- Measuring tube made of Tantalum, Zirconium
- Nominal diameter: DN 8 to 50 ($\frac{3}{8}$ to 2")
- Medium temperature up to +205 °C (+401 °F)
- Remote version with up to 4 I/Os
- Backlit display with touch control and WLAN access
- Standard cable between sensor and transmitter

Your benefits

- Maximum safety for chemically aggressive fluids corrosion-resistant wetted parts
- Fewer process measuring points multivariable measurement (flow, density, temperature)
- Space-saving installation no inlet/outlet run needs
- Full access to process and diagnostic information numerous, freely combinable I/Os and fieldbuses
- Reduced complexity and variety freely configurable I/O functionality
- Integrated verification Heartbeat Technology



Table of contents

| About this document | | Storage temperature | 58 |
|----------------------------------|----|-------------------------------------|----|
| Symbols used | 4 | Climate class | 58 |
| | | Degree of protection | 58 |
| Function and ayetom decign | 5 | Vibration resistance | 58 |
| Function and system design | | Shock resistance | 58 |
| Measuring principle | | Shock resistance | 58 |
| Measuring system | | Interior cleaning | 58 |
| Equipment architecture | | Electromagnetic compatibility (EMC) | 58 |
| Safety | 9 | | |
| | | Process | 58 |
| Input | | Medium temperature range | |
| Measured variable | 11 | Density | 59 |
| Measuring range | 11 | Pressure-temperature ratings | 59 |
| Operable flow range | 12 | Sensor housing | 61 |
| Input signal | 12 | Flow limit | 61 |
| | | Pressure loss | 61 |
| Output | 14 | | 61 |
| | | System pressure | |
| Output and input variants | 15 | Thermal insulation | 62 |
| Output signal | | Heating | |
| Signal on alarm | | Vibrations | bΖ |
| Ex connection data | 21 | | |
| Low flow cut off | 22 | Mechanical construction | 63 |
| | 22 | Dimensions in SI units | 63 |
| Protocol-specific data | 23 | Dimensions in US units | 70 |
| | | Weight | 76 |
| Power supply | 28 | Materials | |
| | 28 | Process connections | |
| Device plugs available | | | 79 |
| Pin assignment, device plug | | | |
| Supply voltage | 31 | 0 1374 | ~~ |
| | 31 | Operability | |
| | 31 | Operating concept | |
| Power supply failure | 31 | Languages | |
| Electrical connection | 32 | Local operation | |
| Potential equalization | 42 | Remote operation | |
| terminals | | | 86 |
| Cable entries | 43 | 5 | 88 |
| Cable specification | | Supported operating tools | |
| cubic specification | 15 | HistoROM data management | 90 |
| Performance characteristics | 48 | | |
| | 48 | Certificates and approvals | 91 |
| | | CE mark | |
| Repeatability | 49 | C-Tick symbol | 91 |
| Response time | 50 | Ex approval | 91 |
| Influence of ambient temperature | 50 | Pharmaceutical compatibility | |
| Influence of medium temperature | | Functional safety | |
| Influence of medium pressure | | HART certification | 94 |
| Design fundamentals | 51 | FOUNDATION Fieldbus certification | |
| Design rundamentals | 51 | Certification PROFIBUS | 95 |
| | | EtherNet/IP certification | 95 |
| Installation | 52 | Certification PROFINET | 95 |
| Mounting location | 52 | Pressure Equipment Directive | 95 |
| Orientation | 53 | Radio approval | 95 |
| Inlet and outlet runs | 54 | Additional certification | 95 |
| | 55 | | 96 |
| Special mounting instructions | 56 | , | |
| | | Ordering information | 96 |
| Environment | 57 | . | _ |
| Ambient temperature range | 57 | | |
| | | | |

2

| Diagnostics functions | 96 97 97 97 97 |
|------------------------------------|----------------------------|
| Communication-specific accessories | 98 98 99 00 |
| Standard documentation | 0 .0 .0 |
| Registered trademarks | 02 |

About this document

$Symbols\ used$

Electrical symbols

| Symbol | Meaning |
|---------------|---|
| | Direct current |
| ~ | Alternating current |
| $\overline{}$ | Direct current and alternating current |
| ± | Ground connection A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system. |
| | Protective Earth (PE) A terminal which must be connected to ground prior to establishing any other connections. |
| | The ground terminals are situated inside and outside the device: Inner ground terminal: Connects the protectiv earth to the mains supply. Outer ground terminal: Connects the device to the plant grounding system. |

Communication symbols

| Symbol | Meaning |
|-------------|---|
| | Wireless Local Area Network (WLAN) Communication via a wireless, local network. |
| • | LED Light emitting diode is off. |
| <u>-</u> \. | LED Light emitting diode is on. |
| | LED Light emitting diode is flashing. |

Symbols for certain types of information

| Symbol | Meaning |
|------------|--|
| ✓ | Permitted Procedures, processes or actions that are permitted. |
| | Preferred Procedures, processes or actions that are preferred. |
| X | Forbidden Procedures, processes or actions that are forbidden. |
| i | Tip Indicates additional information. |
| Ţ <u>i</u> | Reference to documentation. |
| A | Reference to page. |
| | Reference to graphic. |
| | Visual inspection. |

Symbols in graphics

| Symbol | Meaning |
|----------------|--------------------------------|
| 1, 2, 3, | Item numbers |
| 1., 2., 3., | Series of steps |
| A, B, C, | Views |
| A-A, B-B, C-C, | Sections |
| EX | Hazardous area |
| X | Safe area (non-hazardous area) |
| ≋➡ | Flow direction |

Function and system design

Measuring principle

The measuring principle is based on the controlled generation of Coriolis forces. These forces are always present in a system when both translational and rotational movements are superimposed.

 $F_c = 2 \cdot \Delta m (v \cdot \omega)$

 F_c = Coriolis force

 $\Delta m = moving mass$


 ω = rotational velocity

v = radial velocity in rotating or oscillating system

The amplitude of the Coriolis force depends on the moving mass Δm , its velocity v in the system and thus on the mass flow. Instead of a constant rotational velocity ω , the sensor uses oscillation.

In the sensor, an oscillation is produced in the measuring tube. The Coriolis forces produced at the measuring tube cause a phase shift in the tube oscillations (see illustration):

- If there is zero flow (i.e. when the fluid stands still), the oscillation measured at points A and B has the same phase (no phase difference) (1).
- Mass flow causes deceleration of the oscillation at the inlet of the tubes (2) and acceleration at the outlet (3).

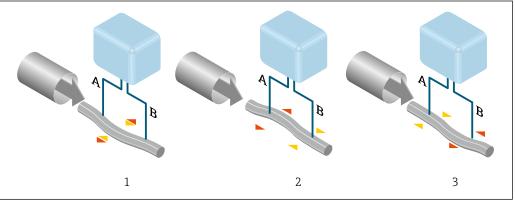

A002993

The phase difference (A-B) increases with increasing mass flow. Electrodynamic sensors register the tube oscillations at the inlet and outlet. System balance is created by exciting an eccentrically arranged swinging mass to antiphase oscillation. The measuring principle operates independently of temperature, pressure, viscosity, conductivity and flow profile.

Density measurement

The measuring tube is continuously excited at its resonance frequency. A change in the mass and thus the density of the oscillating system (comprising measuring tube and fluid) results in a corresponding, automatic adjustment in the oscillation frequency. Resonance frequency is thus a function of medium density. The microprocessor utilizes this relationship to obtain a density signal.

Volume measurement

Together with the measured mass flow, this is used to calculate the volume flow.

Temperature measurement


The temperature of the measuring tube is determined in order to calculate the compensation factor due to temperature effects. This signal corresponds to the process temperature and is also available as an output signal.

Measuring system

The measuring system consists of a transmitter and a sensor. The transmitter and sensor are mounted in physically separate locations. They are interconnected by connecting cables.

Transmitter


Two versions of the transmitter are available.

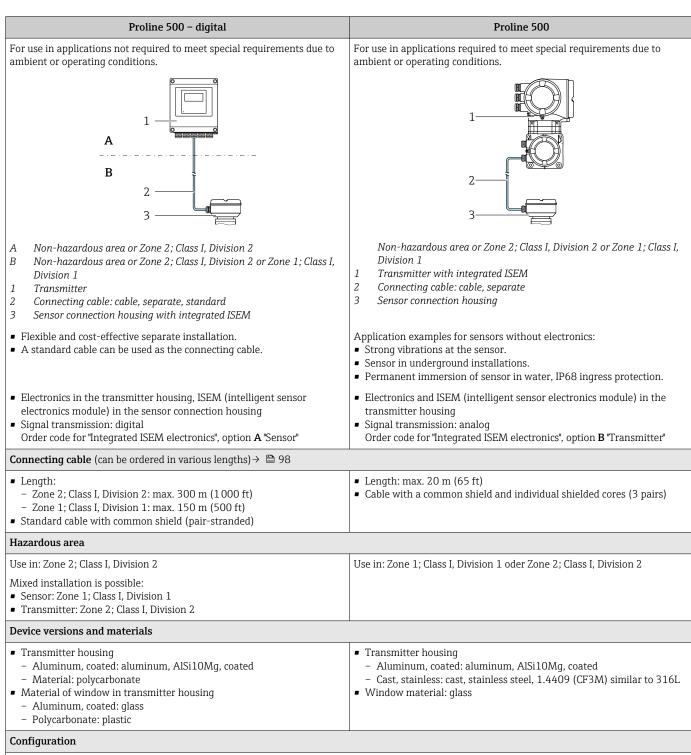


- External operation via 4-line, backlit, graphic local display with touch control and guided menus ("Make-it-run" wizards) for application-specific commissioning.
- Via service interface or WLAN interface:
 - Operating tools (e.g. FieldCare, DeviceCare, SmartBlue app)
 - Web server (access via Web browser, e.g. Microsoft Internet Explorer, Microsoft Edge)

Sensor connection housing

Different versions of the connection housing are available.

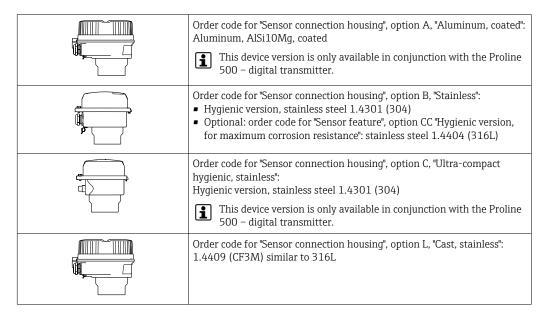


Sensor



- Single bent tube
- Simultaneous measurement of flow, volume flow, density and temperature (multivariable)
- Minimal pressure losses and chemical-resistant materials
- Nominal diameter range: DN 8 to 50 (3/8 to 2")
- Materials:
 - Sensor: stainless steel, 1.4301 (304)
 - Measuring tubes: zirconium 702 (UNS R60702); tantalum 2.5W
 - Process connections: stainless steel, 1.4301 (304), wetted parts: zirconium 702 (UNS R60702); tantalum

Equipment architecture

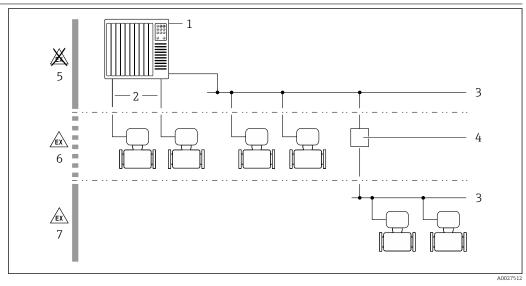

- 1 Possibilities for integrating measuring devices into a system
- 1 Control system (e.g. PLC)
- 2 Connecting cable (0/4 to 20 mA HART etc.)
- 3 Fieldbus
- 4 Segment coupler
- 5 Non-hazardous area
- 6 Hazardous area: Zone 2; Class I, Division 2
- 7 Hazardous area: Zone 1; Class I, Division 1

8

Safety

IT security

Our warranty is valid only if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the device and associated data transfer, must be implemented by the operators themselves in line with their security standards.

Device-specific IT security

The device offers a range of specific functions to support protective measures on the operator's side. These functions can be configured by the user and guarantee greater in-operation safety if used correctly. An overview of the most important functions is provided in the following section.

| Function/interface | Factory setting | Recommendation |
|--|------------------------|---|
| Write protection via hardware write protection switch $\Rightarrow \triangleq 9$ | Not enabled. | On an individual basis following risk assessment. |
| Access code (also applies for Web server login or FieldCare connection) → ■ 9 | Not enabled (0000). | Assign a customized access code during commissioning. |
| WLAN (order option in display module) | Enabled. | On an individual basis following risk assessment. |
| WLAN security mode | Enabled (WPA2- PSK) | Do not change. |
| WLAN passphrase (password) → 🖺 10 | Serial number | Assign a customized access code during commissioning. |
| WLAN mode | Access Point | On an individual basis following risk assessment. |
| Web server→ 🗎 10 | Enabled. | On an individual basis following risk assessment. |
| CDI-RJ45 service interface → 🖺 10 | - | On an individual basis following risk assessment. |

Protecting access via hardware write protection

Write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare) can be disabled via a write protection switch (DIP switch on the motherboard). When hardware write protection is enabled, only read access to the parameters is possible.

Hardware write protection is disabled when the device is delivered.

Protecting access via a password

Different passwords are available to protect write access to the device parameters or access to the device via the WLAN interface.

User-specific access code

Protect write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare). Access authorization is clearly regulated through the use of a user-specific access code.

■ WLAN passphrase

The network key protects a connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option.

Infrastructure mode

When the device is operated in infrastructure mode, the WLAN passphrase corresponds to the WLAN passphrase configured on the operator side.

User-specific access code

Write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare) can be protected by the modifiable, user-specific access code.

WLAN passphrase: Operation as WLAN access point

A connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface, which can be ordered as an optional extra, is protected by the network key. The WLAN authentication of the network key complies with the IEEE 802.11 standard.

When the device is delivered, the network key is pre-defined depending on the device. It can be changed via the **WLAN settings** submenu in the **WLAN passphrase** parameter.

Infrastructure mode

A connection between the device and WLAN access point is protected by means of an SSID and passphrase on the system side. Please contact the relevant system administrator for access.

General notes on the use of passwords

- The access code and network key supplied with the device should be changed during commissioning.
- Follow the general rules for generating a secure password when defining and managing the access code or network key.
- The user is responsible for the management and careful handling of the access code and network key.

Access via Web server

The device can be operated and configured via a Web browser with the integrated Web server. The connection is via the service interface (CDI-RJ45) or the WLAN interface. For device versions with the EtherNet/IP and PROFINET communication protocols, the connection can also be established via the terminal connection for signal transmission with EtherNet/IP or PROFINET (RJ45 connector).

The Web server is enabled when the device is delivered. The Web server can be disabled if necessary (e.g. after commissioning) via the **Web server functionality** parameter.

The device and status information can be hidden on the login page. This prevents unauthorized access to the information.



Access via OPC-UA



The device can communicate with OPC UA clients using the "OPC UA Server" application package.

The OPC UA server integrated in the device can be accessed via the WLAN access point using the WLAN interface - which can be ordered as an optional extra - or the service interface (CDI- RJ45) via Ethernet network. Access rights and authorization as per separate configuration.

The following Security Modes are supported as per the OPC UA Specification (IEC 62541):

- None
- Basic128Rsa15 signed
- Basic128Rsa15 signed and encrypted

Access via service interface (CDI-RJ45)

The device can be connected to a network via the service interface (CDI-RJ45). Device-specific functions quarantee the secure operation of the device in a network.

The use of relevant industrial standards and guidelines that have been defined by national and international safety committees, such as IEC/ISA62443 or the IEEE, is recommended. This includes organizational security measures such as the assignment of access authorization as well as technical measures such as network segmentation.



Input

Measured variable

Direct measured variables

- Mass flow
- Density
- Temperature

Calculated measured variables

- Volume flow
- Corrected volume flow
- Reference density

Measuring range

Measuring range for liquids

| DN | | Measuring range full scale values $\dot{m}_{min(F)}$ to $\dot{m}_{max(F)}$ | |
|------|------|--|------------|
| [mm] | [in] | [kg/h] | [lb/min] |
| 8 | 3/8 | 0 to 2 000 | 0 to 73.50 |
| 15 | 1/2 | 0 to 6 500 | 0 to 238.9 |
| 25 | 1 | 0 to 18 000 | 0 to 661.5 |
| 40 | 11/2 | 0 to 45 000 | 0 to 1654 |
| 50 | 2 | 0 to 70 000 | 0 to 2 573 |

Measuring range for gases

Measuring ranges valid only for Promass H with tantalum 2.5W.

The full scale value depends on the density and the sound velocity of the gas used and can be calculated with the formula below:

 $\dot{m}_{max(G)} = minimum \; (\dot{m}_{max(F)} \cdot \rho_G : x \; ; \; \rho_G \cdot c_G \cdot \pi/2 \cdot (d_i)^2 \cdot 3600)$

| m _{max(G)} | Maximum full scale value for gas [kg/h] |
|---|---|
| m _{max(F)} | Maximum full scale value for liquid [kg/h] |
| $\dot{m}_{\max(G)} < \dot{m}_{\max(F)}$ | $\dot{m}_{ max(G)}$ can never be greater than $\dot{m}_{ max(F)}$ |
| $ ho_{G}$ | Gas density in [kg/m³] at operating conditions |
| х | Constant dependent on nominal diameter |
| c_{G} | Sound velocity (gas) [m/s] |
| d _i | Measuring tube internal diameter [m] |

| DN | | х |
|------|------|---------|
| [mm] | [in] | [kg/m³] |
| 8 | 3/8 | 60 |
| 15 | 1/2 | 80 |
| 25 | 1 | 90 |
| 40 | 1½ | 90 |
| 50 | 2 | 90 |

Recommended measuring range

"Flow limit" section $\rightarrow \triangleq 61$

Operable flow range

Over 1000:1.

Flow rates above the preset full scale value do not override the electronics unit, with the result that the totalizer values are registered correctly.

Input signal


Input and output versions

→ 🖺 14

External measured values

To increase the accuracy of certain measured variables or to calculate the corrected volume flow for gases, the automation system can continuously write different measured values to the measuring device:

- Operating pressure to increase accuracy (Endress+Hauser recommends the use of a pressure measuring device for absolute pressure, e.g. Cerabar M or Cerabar S)
- Medium temperature to increase accuracy (e.g. iTEMP)
- Reference density for calculating the corrected volume flow for gases



It is recommended to read in external measured values to calculate the corrected volume flow.

HART protocol

The measured values are written from the automation system to the measuring device via the HART protocol. The pressure transmitter must support the following protocol-specific functions:

- HART protocol
- Burst mode

Current input

Digital communication

The measured values can be written from the automation system to the measuring via:

- FOUNDATION Fieldbus
- PROFIBUS DP
- PROFIBUS PA
- Modbus RS485
- EtherNet/IP
- PROFINET

Current input 0/4 to 20 mA

| Current input | 0/4 to 20 mA (active/passive) |
|--------------------------|---|
| Current span | 4 to 20 mA (active) 0/4 to 20 mA (passive) |
| Resolution | 1 μΑ |
| Voltage drop | Typically: 0.6 to 2 V for 3.6 to 22 mA (passive) |
| Maximum input voltage | ≤ 30 V (passive) |
| Open-circuit voltage | ≤ 28.8 V (active) |
| Possible input variables | PressureTemperatureDensity |

Status input

| Maximum input values | ■ DC −3 to 30 V ■ If status input is active (ON): R _i >3 kΩ |
|----------------------|--|
| Response time | Adjustable: 5 to 200 ms |
| Input signal level | Low signal: DC -3 to +5 V High signal: DC 12 to 30 V |
| Assignable functions | Off Reset the individual totalizers separately Reset all totalizers Flow override |

Output

Output and input variants

Depending on the option selected for output/input 1, different options are available for the other outputs and inputs. Only one option can be selected for each output/input 1 to 4. The table must be read vertically (\downarrow) .

Example: If the option BA "4-20 mA HART" was selected for output/input 1, one of the options A, B, D, E, F, H, I or J is available for output 2, and one of the options A, B, D, E, F, H, I or J is available for output 3 and 4.

| Order code for "Output; input 1" (020) → | | Possible options | | | | | | | | |
|---|----------|------------------|----------|----------|----------|----------|----------|----------|----|----------|
| Current output 4 to 20 mA HART | BA | | | | | | | | | |
| Current output 4 to 20 mA HART Ex i | 4 | CA | | | | | | | | |
| FOUNDATION Fieldbus | | \ | SA | | | | | | | |
| FOUNDATION Fieldbus Ex i | | | 4 | TA | | | | | | |
| PROFIBUS DP | | | | 4 | LA | | | | | |
| PROFIBUS PA | | | | | + | GA | | | | |
| PROFIBUS PA Ex i | | | | | | 4 | НА | | | |
| Modbus RS485 | | | | | | | \ | MA | | |
| EtherNet/IP 2-port switch integrated | | | | | | | | \ | NA | |
| PROFINET 2-port switch integrated | | | | | | | | | 4 | RA |
| Order code for "Output; input 2" (021) → | 1 | \ | \ | \ | \ | \ | \ | \ | 4 | \ |
| Not assigned | A | Α | Α | Α | A | Α | Α | Α | Α | Α |
| Current output 0/4 to 20 mA | В | | В | | В | В | | В | В | В |
| Current output 0/4 to 20 mA (Ex i) | | С | | С | | | С | | | |
| User configurable input/output 1) | D | | D | | D | D | | D | D | D |
| Pulse/frequency/switch output | Е | | Е | | Е | Е | | Е | Е | E |
| Double pulse output ²⁾ | F | | | | | | | F | | |
| Pulse/frequency/switch output (Ex i) | | G | | G | | | G | | | |
| Relay output | Н | | Н | | Н | Н | | Н | Н | Н |
| Current input 0/4 to 20 mA | I | | I | | I | I | | I | I | I |
| Status input | J | | J | | J | J | | J | J | J |
| Order code for "Output; input 3" (022), "Output; input 4" (023) $^{3)} \rightarrow$ | \ | \ | + | \ | \ | \ | \ | \ | 4 | \ |
| Not assigned | A | Α | Α | Α | Α | Α | Α | A | Α | Α |
| Current output 0/4 to 20 mA | В | | | | В | | | В | В | В |
| Current output 0/4 to 20 mA (Ex i) | | С | | | | | | | | |
| User configurable input/output | D | | | | D | | | D | D | D |
| Pulse/frequency/switch output | Е | | | | Е | | | Е | Е | Е |
| Double pulse output (slave) ^{2) 4)} | F | | | | | | | F | | |
| Pulse/frequency/switch output (Ex i) | | G | | | | | | | | |
| Relay output | Н | | | | Н | | | н | Н | Н |
| Current input 0/4 to 20 mA | I | | | | I | | | I | I | I |
| Status input | J | | | | J | | | J | J | J |

²⁾ If double pulse output (F) is selected for output/input 2 (021), only the double pulse output (F) option is available for selection for output/input 3 (022).

The order code for "Output; input 4" (023) is only available for the Proline 500 – digital transmitter.

⁴⁾ The double pulse output (F) option is not available for input/output 4.

Output signal

HART current output

|) mA (active/passive) |
|--|
| |
| |
| |
| |
| |
| |
| 999 s |
| flow ature acy 0 ag 0 otions increases if the measuring device has one or more |
| |

PROFIBUS PA

| PROFIBUS PA | In accordance with EN 50170 Volume 2, IEC 61158-2 (MBP), galvanically isolated |
|--------------------------|--|
| Data transmission | 31.25 kbit/s |
| Current consumption | 10 mA |
| Permitted supply voltage | 9 to 32 V |
| Bus connection | With integrated reverse polarity protection |

PROFIBUS DP

| Signal encoding | NRZ code |
|-----------------|-------------------|
| Data transfer | 9.6 kBaud12 MBaud |

EtherNet/IP

| Standards | In accordance with IEEE 802.3 |
|-----------|-------------------------------|
|-----------|-------------------------------|

PROFINET

| Standards | In accordance with IEEE 802.3 |
|-----------|-------------------------------|

FOUNDATION Fieldbus

| FOUNDATION Fieldbus | H1, IEC 61158-2, galvanically isolated |
|---------------------|--|
| Data transfer | 31.25 kbit/s |

| Current consumption | 10 mA |
|----------------------------|---|
| Permitted supply voltage | 9 to 32 V |
| Bus connection | With integrated reverse polarity protection |

Modbus RS485

| Physical interface | RS485 in accordance with EIA/TIA-485 standard |
|----------------------|---|
| Terminating resistor | Integrated, can be activated via DIP switches |

Current output 0/4 to 20 mA

| Current output | 0/4 to 20 mA |
|-------------------------------|---|
| Maximum output values | 22.5 mA |
| Current span | Can be set to: 4 to 20 mA (active) 0/4 to 20 mA (passive) Ex-i, passive |
| Open-circuit voltage | DC 28.8 V (active) |
| Maximum input voltage | DC 30 V (passive) |
| Load | 0 to $700~\Omega$ |
| Resolution | 0.38 μΑ |
| Damping | Adjustable: 0.07 to 999 s |
| Assignable measured variables | Mass flow Volume flow Corrected volume flow Density Reference density Temperature Electronic temperature Oscillation frequency 0 Oscillation damping 0 Signal asymmetry Exciter current 0 The range of options increases if the measuring device has one or more application packages. |

Pulse/frequency/switch output

| Function | Can be set to pulse, frequency or switch output |
|------------------------|---|
| Version | Open collector |
| | Can be set to: Active Passive Ex-i, passive |
| Maximum input values | DC 30 V, 250 mA (passive) |
| Open-circuit voltage | DC 28.8 V (active) |
| Voltage drop | For 22.5 mA: ≤ DC 2 V |
| Pulse output | |
| Maximum input values | DC 30 V, 250 mA (passive) |
| Maximum output current | 22.5 mA (active) |

| Open-circuit voltage | DC 28.8 V (active) |
|-------------------------------|--|
| Pulse width | Adjustable: 0.05 to 2 000 ms |
| Maximum pulse rate | 10 000 Impulse/s |
| Pulse value | Adjustable |
| Assignable measured variables | Mass flow Volume flow Corrected volume flow |
| Frequency output | |
| Maximum input values | DC 30 V, 250 mA (passive) |
| Maximum output current | 22.5 mA (active) |
| Open-circuit voltage | DC 28.8 V (active) |
| Output frequency | Adjustable: end value frequency 2 to 10 000 Hz (f _{max} = 12 500 Hz) |
| Damping | Adjustable: 0 to 999 s |
| Pulse/pause ratio | 1:1 |
| Assignable measured variables | Mass flow Volume flow Corrected volume flow Density Reference density Temperature Electronic temperature Oscillation frequency 0 Oscillation damping 0 Signal asymmetry Exciter current 0 The range of options increases if the measuring device has one or more application packages. |
| Switch output | |
| Maximum input values | DC 30 V, 250 mA (passive) |
| Open-circuit voltage | DC 28.8 V (active) |
| Switching behavior | Binary, conductive or non-conductive |
| Switching delay | Adjustable: 0 to 100 s |
| Number of switching cycles | Unlimited |
| Assignable functions | Off On Diagnostic behavior Limit value Mass flow Volume flow Corrected volume flow Density Reference density Temperature Totalizer 1-3 Flow direction monitoring Status Partially filled pipe detection Low flow The range of options increases if the measuring device has one or more application packages. |

Double pulse output

| Function | Double pulse |
|-------------------------------|--|
| Version | Open collector |
| | Can be set to: Active Passive |
| Maximum input values | DC 30 V, 250 mA (passive) |
| Open-circuit voltage | DC 28.8 V (active) |
| Voltage drop | For 22.5 mA: ≤ DC 2 V |
| Output frequency | Adjustable: 0 to 1000 Hz |
| Damping | Adjustable: 0 to 999 s |
| Pulse/pause ratio | 1:1 |
| Assignable measured variables | Mass flow Volume flow Corrected volume flow Density Reference density Temperature The range of options increases if the measuring device has one or more application packages. |

Relay output

| Function | Switch output |
|--------------------------------------|--|
| Version | Relay output, galvanically isolated |
| Switching behavior | Can be set to: NO (normally open), factory setting NC (normally closed) |
| Maximum switching capacity (passive) | DC 30 V, 0.1 A AC 30 V, 0.5 A |
| Assignable functions | ■ Off ■ On ■ Diagnostic behavior ■ Limit value ■ Mass flow ■ Volume flow ■ Corrected volume flow ■ Density ■ Reference density ■ Temperature ■ Totalizer 1-3 ■ Flow direction monitoring ■ Status ■ Partially filled pipe detection ■ Low flow The range of options increases if the measuring device has one or more application packages. |

User configurable input/output

 $\textbf{One} \ specific input or output is assigned to a user-configurable input/output (configurable I/O) during device commissioning.$

The following inputs and outputs are available for assignment:

- Choice of current output: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Pulse/frequency/switch output
- Choice of current input: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Status input

The technical values correspond to those of the inputs and outputs described in this section.

Signal on alarm

Depending on the interface, failure information is displayed as follows:

HART current output

| Device diagnostics | Device condition can be read out via HART Command 48 |
|--------------------|--|
| Device diagnostics | Device condition can be read out via HART Command 48 |

PROFIBUS PA

| Status and alarm messages | Diagnostics in accordance with PROFIBUS PA Profile 3.02 |
|--|---|
| Failure current FDE (Fault Disconnection Electronic) | 0 mA |

PROFIBUS DP

| Status and alarm | Diagnostics in accordance with PROFIBUS PA Profile 3.02 |
|------------------|---|
| messages | |

EtherNet/IP

| Device diagnostics | Device condition can be read out in Input Assembly |
|--------------------|--|
|--------------------|--|

PROFINET

| Device diagnostics | According to "Application Layer protocol for decentralized periphery", Version 2.3 |
|--------------------|--|
|--------------------|--|

FOUNDATION Fieldbus

| Status and alarm messages | Diagnostics in accordance with FF-891 |
|--|---------------------------------------|
| Failure current FDE (Fault Disconnection Electronic) | 0 mA |

Modbus RS485

| Failure mode | Choose from: |
|--------------|--------------------------------------|
| | ■ NaN value instead of current value |
| | ■ Last valid value |

Current output 0/4 to 20 mA

4 to 20 mA

| Choose from: 4 to 20 mA in accordance with NAMUR recommendation NE 43 4 to 20 mA in accordance with US Min. value: 3.59 mA Max. value: 22.5 mA Freely definable value between: 3.59 to 22.5 mA Actual value Last valid value |
|---|
|---|

0 to 20 mA

| Failure mode | Choose from: |
|--------------|--|
| | ■ Maximum alarm: 22 mA |
| | ■ Freely definable value between: 0 to 20.5 mA |

Pulse/frequency/switch output

| Pulse output | |
|------------------|--|
| Failure mode | Choose from: Actual value No pulses |
| Frequency output | |
| Failure mode | Choose from: Actual value O Hz Defined value (f max 2 to 12 500 Hz) |
| Switch output | |
| Failure mode | Choose from: Current status Open Closed |

Relay output

| Failure mode | Choose from: Current status |
|--------------|---------------------------------------|
| | OpenClosed |

Local display

| Plain text display | With information on cause and remedial measures |
|--------------------|---|
| Backlight | Red backlighting indicates a device error. |



Status signal as per NAMUR recommendation NE 107

Interface/protocol

- Via digital communication:
 - HART protocol
 - FOUNDATION Fieldbus
 - PROFIBUS PA
 - PROFIBUS DP
 - Modbus RS485
 - EtherNet/IP
 - PROFINET
- Via service interface
 - CDI-RJ45 service interface
 - WLAN interface

| Plain text display | With information on cause and remedial measures |
|--------------------|---|
|--------------------|---|



Web server

| Plain text display | With information on cause and remedial measures |
|--------------------|---|
|--------------------|---|

Light emitting diodes (LED)

| Status information | Status indicated by various light emitting diodes |
|--------------------|--|
| | The following information is displayed depending on the device version: Supply voltage active Data transmission active Device alarm/error has occurred EtherNet/IP network available EtherNet/IP connection established PROFINET network available PROFINET connection established PROFINET blinking feature |

Ex connection data

Safety-related values

| Order code for "Output; input 1" | Output type | Safety-related values "Output; input 1" | | | |
|----------------------------------|-----------------------------------|--|--------|--|--|
| | | 26 (+) | 27 (-) | | |
| Option BA | Current output 4 to 20 mA HART | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option GA | PROFIBUS PA | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option LA | PROFIBUS DP | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option MA | Modbus RS485 | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option SA | FOUNDATION Fieldbus | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option NA | EtherNet/IP | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |
| Option RA | PROFINET | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | |

| Order code for | Output type | Safety-related values | | | | | | |
|--|--------------------------------|--|--------|-----------------|--------|--------------|--------|--|
| "Output; input 2"; "Output; input 3" "Output; input 4" | | Output; input 2 | | Output; input 3 | | Output; inpu | | |
| | | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) | |
| Option B | Current output 4 to 20 mA | $U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$ | | | | | | |
| Option D | User configurable input/output | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | | | | |
| Option E | Pulse/frequency/switch output | $U_{N} = 30 V_{DC}$ $U_{M} = 250 V_{AC}$ | | | | | | |
| Option F | Double pulse output | $U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$ | | | | | | |
| Option H | Relay output | $U_{N} = 30 V_{DC}$ $I_{N} = 100 \text{ mA}_{DC} / 500 \text{ mA}_{AC}$ $U_{M} = 250 V_{AC}$ | | | | | | |

| Order code for | Output type | Output type Safety-related values | | | s | | |
|--|-----------------------------|---|--------------------------------------|---------|-----------------|--------|------------------|
| "Output; input 2"; "Output; input 3" "Output; input 4" | | Output; input 2 | | Output; | Output; input 3 | | t ; input |
| 1 / 1 | | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) |
| Option I | Current input 4 to 20 mA | $U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$ | | | | | |
| Option J | Status input | $U_{\rm N} = 30$ $V_{\rm M} = 250$ | V _{DC}) V _{AC} | | | | |

The order code "Output; input 4" is only available for the Proline 500 – digital transmitter.

Intrinsically safe values

| Order code for "Output; input 1" | Output type | Intrinsically safe values "Output; input 1" | | | | |
|----------------------------------|--|--|--|--|--|--|
| | | 26 (+) | 27 (-) | | | |
| Option CA | Current output 4 to 20 mA HART Ex i | $\begin{split} &U_{i} = 30 \text{ V} \\ &l_{i} = 100 \text{ mA} \\ &P_{i} = 1.25 \text{ W} \\ &L_{i} = 0 \\ &C_{i} = 0 \end{split}$ | | | | |
| Option HA | PROFIBUS PA Ex i | Ex ia $^{1)}$ $U_i = 30 \text{ V}$ $l_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ | Ex ic 2) $U_{i} = 32 \text{ V}$ $l_{i} = 570 \text{ mA}$ $P_{i} = 8.5 \text{ W}$ $L_{i} = 10 \mu\text{H}$ $C_{i} = 5 \text{ nF}$ | | | |
| Option TA | FOUNDATION Fieldbus Ex i | $\begin{aligned} \textbf{Ex ia}^{\ 1)} \\ U_i &= 30 \text{ V} \\ l_i &= 570 \text{ mA} \\ P_i &= 8.5 \text{ W} \\ L_i &= 10 \mu\text{H} \\ C_i &= 5 \text{ nF} \end{aligned}$ | Ex ic ²⁾ $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \mu\text{H}$ $C_i = 5 \text{ nF}$ | | | |

- 1) 2) Only available for the Zone 1; Class I, Division 1 version
- Only available for the Zone 2; Class I, Division 2 version and only for the Proline 500 digital transmitter

| Order code for | Output type Intrinsically safe values or NIFW values | | | | s | | |
|--------------------------------------|--|--|--------|--------------------|--------|--------|--------|
| "Output; input 2"; "Output; input 3" | | Output; input 2 Output; input 3 Output | | Output; input 4 1) | | | |
| "Output; input 4" | | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) |
| Option C | Current output 4 to 20 mA Ex i | $\begin{aligned} &U_i = 30 \text{ V} \\ &l_i = 100 \text{ r} \\ &P_i = 1.25 \\ &L_i = 0 \\ &C_i = 0 \end{aligned}$ | nA | | | | |
| Option G | Pulse/frequency/switch output Ex i | $\begin{aligned} &U_i = 30 \text{ V} \\ &l_i = 100 \text{ r} \\ &P_i = 1.25 \\ &L_i = 0 \\ &C_i = 0 \end{aligned}$ | nA | | | | |

1) The order code "Output; input 4" is only available for the Proline 500- digital transmitter.

Low flow cut off

The switch points for low flow cut off are user-selectable.

Galvanic isolation

The outputs are galvanically isolated from one another and from earth (PE).

Protocol-specific data

HART

| Manufacturer ID | 0x11 |
|------------------------------------|--|
| Device type ID | 0x3B |
| HART protocol revision | 7 |
| Device description files (DTM, DD) | Information and files under: www.endress.com |
| HART load | Min. 250 Ω |
| System integration | Information on system integration: Operating Instructions → 🗎 101. • Measured variables via HART protocol • Burst Mode functionality |

PROFIBUS PA

| Manufacturer ID | 0x11 |
|---|--|
| Ident number | 0x156D |
| Profile version | |
| | 3.02 |
| Device description files (GSD, DTM, DD) | Information and files under: www.endress.com www.profibus.org |
| Supported functions | Identification & Maintenance Simplest device identification on the part of the control system and nameplate PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur |
| Configuration of the device address | DIP switches on the I/O electronics module Local display Via operating tools (e.g. FieldCare) |
| Compatibility with earlier model | If the device is replaced, the measuring device Promass 500 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 500 GSD file. |
| | Earlier models: Promass 80 PROFIBUS PA ID No.: 1528 (hex) Extended GSD file: EH3x1528.gsd Standard GSD file: EH3_1528.gsd Promass 83 PROFIBUS PA ID No.: 152A (hex) Extended GSD file: EH3x152A.gsd Standard GSD file: EH3x152A.gsd |
| | Description of the function scope of compatibility: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ |
| System integration | Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ |
| | Cyclic data transmission Block model Description of the modules |

PROFIBUS DP

| Manufacturer ID | 0x11 |
|-----------------|--------|
| Ident number | 0x156F |

| Profile version | 3.02 |
|---|--|
| Device description files (GSD, DTM, DD) | Information and files under: ■ www.endress.com On the product page for the device: Documents/Software → Device drivers ■ www.profibus.org |
| Supported functions | Identification & Maintenance Simplest device identification on the part of the control system and nameplate PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur |
| Configuration of the device address | DIP switches on the I/O electronics module Via operating tools (e.g. FieldCare) |
| Compatibility with earlier model | If the device is replaced, the measuring device Promass 500 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promass 500 GSD file. |
| | Previous model: Promass 83 PROFIBUS DP - ID No.: 1529 (hex) - Extended GSD file: EH3x1529.gsd - Standard GSD file: EH3_1529.gsd Description of the function scope of compatibility: Operating Instructions → ■ 101. |
| System integration | Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ |
| | Cyclic data transmission Block model Description of the modules |

EtherNet/IP

| Protocol | The CIP Networks Library Volume 1: Common Industrial Protocol The CIP Networks Library Volume 2: EtherNet/IP Adaptation of CIP |
|--|---|
| Communication type | ■ 10Base-T ■ 100Base-TX |
| Device profile | Generic device (product type: 0x2B) |
| Manufacturer ID | 0x11 |
| Device type ID | 0x103B |
| Baud rates | Automatic $^{10}\!\!/_{100}$ Mbit with half-duplex and full-duplex detection |
| Polarity | Auto-polarity for automatic correction of crossed TxD and RxD pairs |
| Supported CIP connections | Max. 3 connections |
| Explicit connections | Max. 6 connections |
| I/O connections | Max. 6 connections (scanner) |
| Configuration options for measuring device | DIP switches on the electronics module for IP addressing Manufacturer-specific software (FieldCare) Add-on Profile Level 3 for Rockwell Automation control systems Web browser Electronic Data Sheet (EDS) integrated in the measuring device |
| Configuration of the EtherNet interface | Speed: 10 MBit, 100 MBit, auto (factory setting) Duplex: half-duplex, full-duplex, auto (factory setting) |

| Configuration of the device address | DIP switches on the electronics module for IP addressing (last octet) DHCP Manufacturer-specific software (FieldCare) Add-on Profile Level 3 for Rockwell Automation control systems Web browser EtherNet/IP tools, e.g. RSLinx (Rockwell Automation) | | | |
|-------------------------------------|--|--|--|--|
| Device Level Ring (DLR) | Yes | | | |
| System integration | Information regarding system integration: Operating Instructions $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ | | | |
| | Cyclic data transmission Block model Input and output groups | | | |

PROFINET

| Protocol | "Application layer protocol for decentral device periphery and distributed automation", version 2.3 |
|--|--|
| Communication type | 100 MBit/s |
| Conformity class | Conformance Class B |
| Netload Class | Netload Class II |
| Baud rates | Automatic 100 Mbit/s with full-duplex detection |
| Cycle times | From 8 ms |
| Polarity | Auto-polarity for automatic correction of crossed TxD and RxD pairs |
| Media Redundancy Protocol (MRP) | Yes |
| Device profile | Application interface identifier 0xF600 Generic device |
| Manufacturer ID | 0x11 |
| Device type ID | 0x843B |
| Device description files (GSD, DTM, DD) | Information and files under: ■ www.endress.com On the product page for the device: Documents/Software → Device drivers ■ www.profibus.org |
| Supported connections | 1 x AR (IO Controller AR) 1 x AR (IO-Supervisor Device AR connection allowed) 1 x Input CR (Communication Relation) 1 x Output CR (Communication Relation) 1 x Alarm CR (Communication Relation) |
| Configuration options for measuring device | DIP switches on the electronics module, for device name assignment (last part) Manufacturer-specific software (FieldCare, DeviceCare) Web browser Device master file (GSD), can be read out via the integrated Web server of the measuring device |
| Configuration of the device name | DIP switches on the electronics module, for device name assignment (last part) DCP protocol Process Device Manager (PDM) Integrated Web server |

| Supported functions | Identification & Maintenance Simple device identification via: |
|---------------------|--|
| System integration | Information regarding system integration: Operating Instructions → 🗎 101. Cyclic data transmission Overview and description of the modules Status coding Startup configuration Factory setting: |

FOUNDATION Fieldbus

| Manufacturer ID | 0x452B48 (hex) | | | | | | |
|---------------------------------|--|--|--|--|--|--|--|
| Ident number | 0x103B (hex) | | | | | | |
| Device revision | 1 | | | | | | |
| | | | | | | | |
| DD revision | Information and files under: www.endress.com | | | | | | |
| CFF revision | • www.fieldbus.org | | | | | | |
| Interoperability Test Kit (ITK) | Version 6.2.0 | | | | | | |
| ITK Test Campaign Number | Information: | | | | | | |
| | www.endress.comwww.fieldbus.orq | | | | | | |
| Link Master capability (LAS) | Yes | | | | | | |
| Choice of "Link Master" and | Yes | | | | | | |
| "Basic Device" | Factory setting: Basic Device | | | | | | |
| Node address | Factory setting: 247 (0xF7) | | | | | | |
| Supported functions | The following methods are supported: Restart ENP Restart Diagnostic Set to OOS Set to AUTO Read trend data Read event logbook | | | | | | |
| Virtual Communication Relation | onships (VCRs) | | | | | | |
| Number of VCRs | 44 | | | | | | |
| Number of link objects in VFD | 50 | | | | | | |
| Permanent entries | 1 | | | | | | |
| Client VCRs | 0 | | | | | | |
| Server VCRs | 10 | | | | | | |
| Source VCRs | 43 | | | | | | |
| Sink VCRs | 0 | | | | | | |
| Subscriber VCRs | 43 | | | | | | |
| Publisher VCRs | 43 | | | | | | |
| Device Link Capabilities | | | | | | | |
| Slot time | 4 | | | | | | |
| Min. delay between PDU | 8 | | | | | | |

| Max. response delay | 16 |
|---------------------|--|
| System integration | Information regarding system integration: Operating Instructions → 🗎 101. Cyclic data transmission Description of the modules Execution times Methods |

Modbus RS485

| Protocol | Modbus Applications Protocol Specification V1.1 |
|----------------------------------|--|
| Response times | Direct data access: typically 25 to 50 ms Auto-scan buffer (data range): typically 3 to 5 ms |
| Device type | Slave |
| Slave address range | 1 to 247 |
| Broadcast address range | 0 |
| Function codes | 03: Read holding register 04: Read input register 06: Write single registers 08: Diagnostics 16: Write multiple registers 23: Read/write multiple registers |
| Broadcast messages | Supported by the following function codes: O6: Write single registers 16: Write multiple registers 23: Read/write multiple registers |
| Supported baud rate | 1200 BAUD 2400 BAUD 4800 BAUD 9600 BAUD 19200 BAUD 38400 BAUD 57600 BAUD 115200 BAUD |
| Data transfer mode | ■ ASCII ■ RTU |
| Data access | Each device parameter can be accessed via Modbus RS485. For Modbus register information |
| Compatibility with earlier model | If the device is replaced, the measuring device Promass 500 supports the compatibility of the Modbus registers for the process variables and the diagnostic information with the previous model Promass 83. It is not necessary to change the engineering parameters in the automation system. □ Description of the function scope of compatibility: Operating Instructions → ■ 101. |
| System integration | Information on system integration: Operating Instructions → 🗎 101. ■ Modbus RS485 information ■ Function codes ■ Register information ■ Response time ■ Modbus data map |

Power supply

Terminal assignment

Transmitter: supply voltage, input/outputs

HART

| Supply | Supply voltage | | output l | Input/output 2 | | Input/output 3 | | Input/output 4 | |
|--------|----------------|---|-------------|-------------------|--------|-------------------|--------|-------------------|--------|
| 1 (+) | 2 (-) | 26 (+) | 27 (-) | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) |
| | | The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ | | | | | | | |

FOUNDATION Fieldbus

| Supply voltage | | Input/output 1 | | Input/output 2 | | Input/ | output 3 | Input/ | output i |
|----------------|-------|---|--------|----------------|--------|--------|-------------|--------|------------------------|
| 1 (+) | 2 (-) | 26 (A) | 27 (B) | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) |
| | | The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ | | | | | | | |

PROFIBUS PA

| Supply voltage | | Input/output 1 | | Input/output 2 | | Input/ | output 3 | Input/ | output 1 |
|----------------|-------|---|--------|-------------------|--------|--------|-------------|--------|------------------------|
| 1 (+) | 2 (-) | 26 (B) | 27 (A) | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) |
| | | The terminal assignment depends on the specific device version ordered $ ightarrow$ $ ightharpoons$ 14. | | | | | | | |

PROFIBUS DP

| Supply voltage | | Input/ | output l | Input/output 2 | | Input/output 3 | | Input/output 4 | | | |
|----------------|-------|--------|--|-------------------|--------|-------------------|--------|----------------|--------|--|--|
| 1 (+) | 2 (-) | 26 (B) | 27 (A) | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) | | |
| | | The t | The terminal assignment depends on the specific device version ordered → 🖺 14. | | | | | | | | |

Modbus RS485

| Supply | Supply voltage Input/output 1 | | Input/output 2 | | Input/output 3 | | Input/output 4 | | | | | |
|--------|-------------------------------|--------|--|--------|-------------------|--------|----------------|--------|--------|--|--|--|
| 1 (+) | 2 (-) | 26 (B) | 27 (A) | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) | | | |
| | | The t | The terminal assignment depends on the specific device version ordered → 🗎 14. | | | | | | | | | |

PROFINET

| Supply | Supply voltage Input/ou 1 | | Input/output 2 | | Input/output 3 | | Input/output 4 | | |
|--------|------------------------------|------------------|---|--------|-------------------|--------|----------------|--------|--|
| 1 (+) | 2 (-) | PROFINET | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) | |
| | | (RJ45 connector) | The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ | | | | | | |

EtherNet/IP

| Supply voltage | | Input/output 1 | Input/output 2 | | Input/output 3 | | Input/output 4 | | |
|----------------|-------|-------------------|---|--------|----------------|--------|----------------|--------|--|
| 1 (+) | 2 (-) | EtherNet/IP | 24 (+) | 25 (-) | 22 (+) | 23 (-) | 20 (+) | 21 (-) | |
| | | (RJ45 connector) | The terminal assignment depends on the specific device version ordered $\rightarrow \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ $ | | | | | | |

Transmitter and sensor connection housing: connecting cable

The sensor and transmitter, which are mounted in separate locations, are interconnected by a connecting cable. The cable is connected via the sensor connection housing and the transmitter housing.

Terminal assignment and connection of the connecting cable:

- Proline 500 digital → 32
- Proline 500 → 🖺 32

Device plugs available



Device plugs may not be used in hazardous areas!

Device plugs for fieldbus systems:

Order code for "Input; output 1"

- Option **SA** "FOUNDATION Fieldbus" → 🖺 29
- Option **GA** "PROFIBUS PA" → 🗎 29
- Option RA "PROFINET" →

 29
- Option **NA** "EtherNet/IP" → 🗎 29

Device plug for connecting to the service interface:

Order code for "Accessory mounted"

option NB, adapter RJ45 M12 (service interface) → 🖺 31

Order code for "Input; output 1", option SA "FOUNDATION Fieldbus"

| | Order code for | Cable entry/connection → 🗎 33 | | | | |
|-------------------------|----------------|-------------------------------|---|--|--|--|
| "Electrical connection" | | 2 | 3 | | | |
| | M, 3, 4, 5 | 7/8" connector | - | | | |

Order code for "Input; output 1", option GA "PROFIBUS PA"

| Order code for | Cable entry/connection → 🖺 33 | | | |
|-------------------------|-------------------------------|---|--|--|
| "Electrical connection" | 2 | 3 | | |
| L, N, P, U | Connector M12 × 1 | - | | |

Order code for "Input; output 1", option RA "PROFINET"

| Order code for | Cable entry/connection → 🖺 33 | | | |
|---|-------------------------------|-------------------|--|--|
| "Electrical connection" | 2 | 3 | | |
| L, N, P, U | Connector M12 × 1 | _ | | |
| R ¹⁾²⁾ , S ¹⁾²⁾ , T ¹⁾²⁾ , V ¹⁾²⁾ | Connector M12 × 1 | Connector M12 × 1 | | |

- Cannot be combined with an external WLAN antenna (order code for "Enclosed accessories", option P8) of an RJ45 M12 adapter for the service interface (order code for "Accessories mounted", option NB) or of the remote display and operating module DKX001.
- 2) Suitable for integrating the device in a ring topology.

Order code for "Input; output 1", option NA "EtherNet/IP"

| Order code for | Cable entry/connection → 🗎 33 | | | | |
|---|-------------------------------|-------------------|--|--|--|
| "Electrical connection" | 2 | 3 | | | |
| L, N, P, U | Connector M12 × 1 | - | | | |
| R ¹⁾²⁾ , S ¹⁾²⁾ , T ¹⁾²⁾ , V ¹⁾²⁾ | Connector M12 × 1 | Connector M12 × 1 | | | |

- Cannot be combined with an external WLAN antenna (order code for "Enclosed accessories", option P8) of an RJ45 M12 adapter for the service interface (order code for "Accessories mounted", option NB) or of the remote display and operating module DKX001
- 2) Suitable for integrating the device in a ring topology.

Order code for "Accessory mounted", option NB "Adapter RJ45 M12 (service interface)"

| Order code | Cable entry/coupling → 🖺 33 | | | |
|---------------------|-----------------------------|------------------|--|--|
| "Accessory mounted" | Cable entry 2 | Cable entry 3 | | |
| NB | Plug M12 × 1 | - | | |

Pin assignment, device plug


FOUNDATION Fieldbus

| | Pin | | Assignment | Coding | Plug/socket |
|-------|-----|---|--------------|--------|-------------|
| 2 () | 1 | + | Signal + | А | Plug |
| | 2 | - | Signal – | | |
| | 3 | | Grounding | | |
| | 4 | | Not assigned | | |

PROFIBUS PA

| | Pin | | Assignment | Coding | Plug/socket |
|-------------|-------|---|---------------|--------|-------------|
| 2 / 3 | 1 | + | PROFIBUS PA + | A | Plug |
| 1 4 | 1 4 2 | | Grounding | | |
| \frac{1}{2} | 3 | - | PROFIBUS PA - | | |
| | 4 | | Not assigned | | |


PROFINET

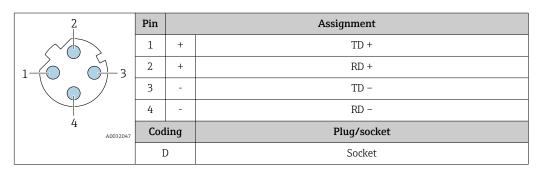



- Recommended plug:
 Binder, series 763, part no. 99 3729 810 04
 - Phoenix, part no. 1543223 SACC-M12MSD-4Q
 - When using the device in a hazardous location, use a suitably certified plug.

EtherNet/IP

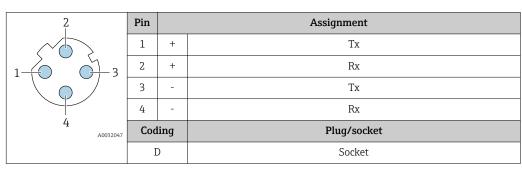


- Recommended plug:
 Binder, series 763, part no. 99 3729 810 04
 - Phoenix, part no. 1543223 SACC-M12MSD-4Q
 - When using the device in a hazardous location, use a suitably certified plug.

30

Service interface

Order code for "Accessories mounted", option NB: Adapter RJ45 M12 (service interface)

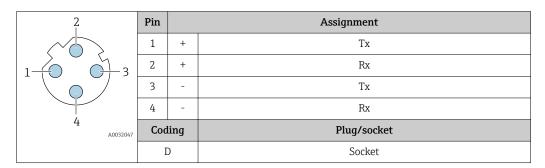



Recommended plug:

- Binder, series 763, part no. 99 3729 810 04
- Phoenix, part no. 1543223 SACC-M12MSD-4Q
- When using the device in a hazardous location, use a suitably certified plug.

Supply voltage

| Order code for "Power supply" | terminal voltage | | Frequency range |
|----------------------------------|------------------|---------|-----------------|
| Option D | DC24 V | ±20% | - |
| Option E | AC100 to 240 V | -15+10% | 50/60 Hz |
| Option I | DC24 V | ±20% | - |
| Option I | AC100 to 240 V | -15+10% | 50/60 Hz |

Power consumption

Transmitter

Max. 10 W (active power)

| switch-on current | Max. 36 A (as per NAMUR Recommendation NE21) |
|-------------------|--|
|-------------------|--|

Current consumption

Transmitter


- Max. 400 mA (24 V)
- Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)

Power supply failure

- Totalizers stop at the last value measured.
- Depending on the device version, the configuration is retained in the device memoryor in the pluggable data memory (HistoROM DAT).
- Error messages (incl. total operated hours) are stored.

Electrical connection

Connection of connecting cable: Proline 500 - digital

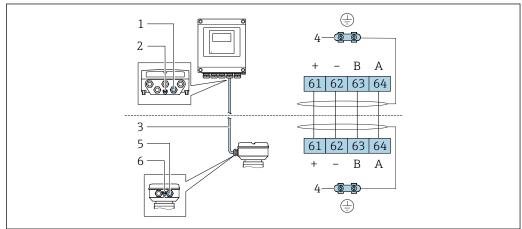

A002819

- 1 Cable entry for cable on transmitter housing
- 2 Protective ground (PE)
- 3 Connecting cable ISEM communication
- 4 Grounding via ground connection; on device plug versions grounding is through the plug itself
- 5 Cable entry for cable or connection of device plug on sensor connection housing
- *6 Protective ground (PE)*

Depending on the device version of the sensor connection housing, the connecting cable is connected via terminals or device plugs.

| Sensor connection housing Order code for "Housing" | Connection to sensor connection housing via | Connection to transmitter housing via | |
|---|---|---|--|
| Option A : aluminum coated | Terminals | Terminals | |
| Option B : stainless | Terminals | Terminals | |
| Option C ultra-compact, hygienic, stainless | Device plug | Terminals | |

Pin assignment, device plug

Device plugs are only available for device version, order code for "Housing":

Option **C** ultra-compact, hygienic, stainless

For connection to sensor connection housing.

| 3 1 5 | Pin | Color 1) | Assignment | | Connection to terminal |
|-------|--------|----------|------------|---------------------|------------------------|
| | 1 | Brown | + | Supply voltage | 61 |
| | 2 | White | А | ISEM communication | 64 |
| | 3 | Blue | В | ISENI COMMUNICATION | 04 |
| | 4 | Black | - | Supply voltage | 63 |
| | 5 | - | | - | 62 |
| | Coding | | | Plug/socket | |
| A | | | Plug | | |


1) Cable colors of connecting cable

A connecting cable with a device plug is optionally available.

Connection of the connecting cable: Proline 500

The connecting cable is connected via terminals.

32

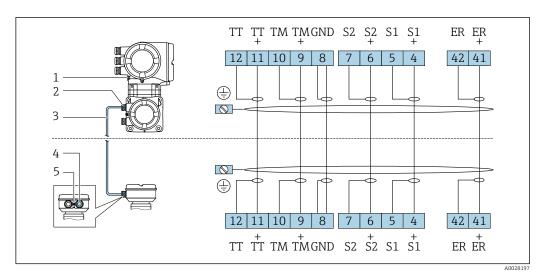

Protective ground (PE)


- 2 Cable entry for connecting cable on transmitter connection housing
- 3 Connecting cable
- Cable entry for connecting cable on sensor connection housing
- Protective ground (PE)

Connecting the transmitter



- Terminal assignment → 🖺 28
- Device plug pin assignment → 🖺 30

Connecting the Proline 500 - digital transmitter

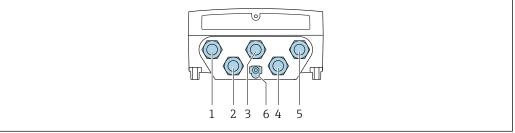


- Terminal connection for supply voltage
- Terminal connection for signal transmission, input/output
- Terminal connection for signal transmission, input/output
- Terminal connection for connecting cable between sensor and transmitter
- Terminal connection for signal transmission, input/output or terminal for network connection (DHCP client) via service interface (CDI-RJ45); optional: terminal connection for external WLAN antenna
- Protective ground (PE)
- An adapter for RJ45 and the M12 plug is optionally available: Order code for "Accessories", option NB: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. Therefore the connection to the service interface can be established via an M12connector without opening the device.

Network connection (DHCP client) via service interface (CDI-RJ45) → 🖺 86

Connecting the Proline 500 transmitter

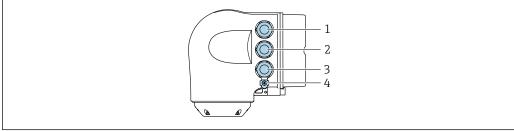

- Terminal connection for supply voltage
- Terminal connection for signal transmission, input/output
- Terminal connection for signal transmission, input/output or terminal for network connection (DHCP client) 3 via service interface (CDI-RJ45); optional: terminal connection for external WLAN antenna
- Protective ground (PE)
- An adapter for RJ45 and the M12 plug is optionally available: Order code for "Accessories", option NB: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. Therefore the connection to the service interface can be established via an M12 connector without opening the device.


Network connection (DHCP client) via service interface (CDI-RJ45) → 🖺 86

Connecting in a ring topology

Device versions with EtherNet/IP and PROFINET communication protocols can be integrated into a ring topology. The device is integrated via the terminal connection for signal transmission (output 1) and the connection to the service interface (CDI-RJ45).


- Integrating the transmitter into a ring topology:
 - EtherNet/IP → 🖺 84
 - PROFINET → 🖺 85

Transmitter: Proline 500 - digital

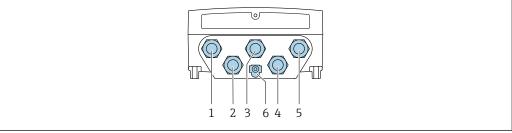

- Terminal connection for supply voltage
- Terminal connection for signal transmission, input/output 2
- Terminal connection for signal transmission: PROFINET or EtherNet/IP (RJ45 connector)
- 4 Terminal connection for connecting cable between sensor and transmitter
- Terminal connection to service interface (CDI-RJ45)
- Protective ground (PE)

Transmitter: Proline 500

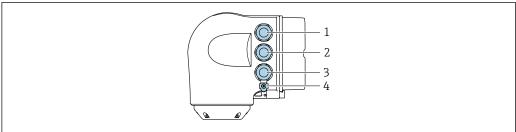


- Terminal connection for supply voltage
- Terminal connection for signal transmission: PROFINET or EtherNet/IP (RJ45 connector) 2
- 3 Terminal connection to service interface (CDI-RJ45)
- Protective ground (PE)


If the device has additional inputs/outputs, these are routed in parallel via the cable entry for connection to the service interface (CDI-RJ45).

Connection examples

Current output 4 to 20 mA HART

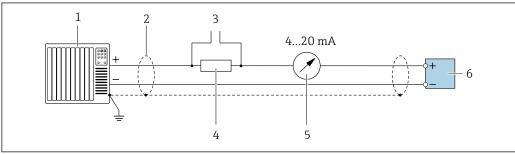


- **№** 2 Connection example for 4 to 20 mA HART current output (active)
- Automation system with current input (e.g. PLC) 1
- 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable $specifications \rightarrow \implies 43$
- Connection for HART operating devices $\rightarrow \blacksquare 81$
- 4
- Analog display unit: observe maximum load $\rightarrow \blacksquare 15$
- Transmitter

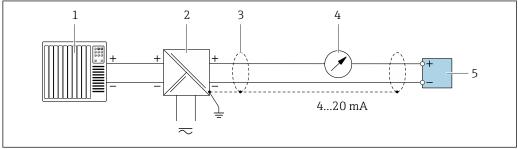

- **₽** 3 Connection example for 4 to 20 mA HART current output (passive)
- Automation system with current input (e.g. PLC)
- Power supply 2
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable $specifications \rightarrow \implies 43$
- Analog display unit: observe maximum load → 🖺 15
- Transmitter


HART input

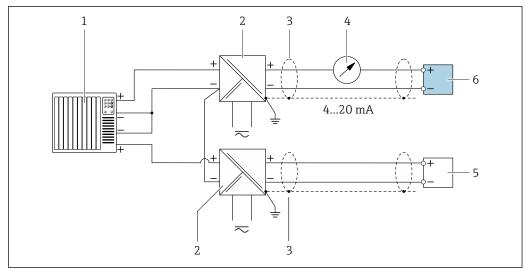

A002876

- 4 Connection example for HART input with a common negative (passive)
- 1 Automation system with HART output (e.g. PLC)
- 2 Active barrier for power supply (e.g. RN221N)
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 Analog display unit: observe maximum load
- 5 Pressure transmitter (e.g. Cerabar M, Cerabar S): see requirements
- 6 Transmitter

PROFIBUS PA

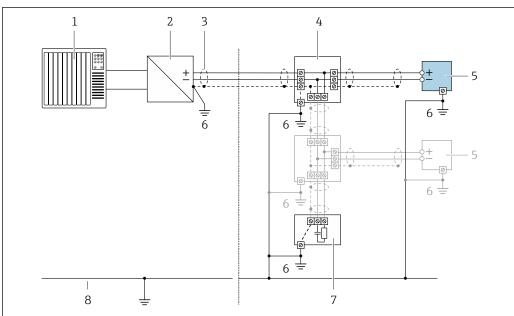


A002876

■ 5 Connection example for PROFIBUS PA


- 1 Control system (e.g. PLC)
- 2 PROFIBUS PA segment coupler
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 T-box
- 5 Measuring device
- 6 Local grounding
- 7 Bus terminator
- 8 Potential matching line

PROFIBUS DP

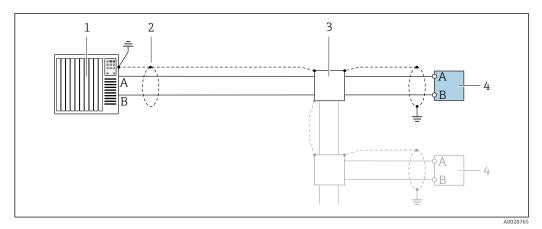

- \blacksquare 6 Connection example for PROFIBUS DP, non-hazardous area and Zone 2/Div. 2
- 1 Control system (e.g. PLC)
- 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 3 Distribution box
- 4 Transmitter
- If baud rates > 1.5 MBaud an EMC cable entry must be used and the cable shield must continue as far as the terminal wherever possible.


EtherNet/IP

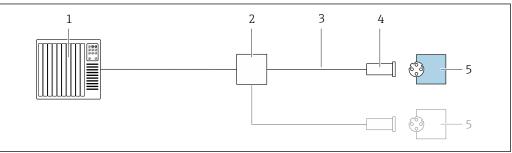

A002876


- 7 Connection example for EtherNet/IP
- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications
- 4 Device plug
- 5 Transmitter

EtherNet/IP: DLR (Device Level Ring)

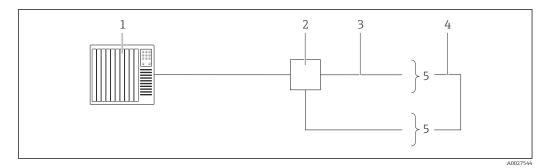

- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3
- Connecting cable between the two transmitters
- Transmitter


PROFINET

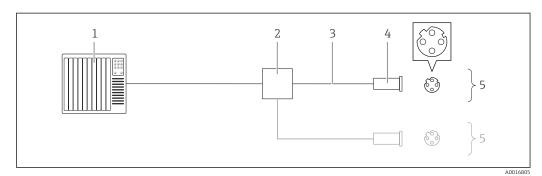

₽8 Connection example for PROFINET


- Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications
- 4 Device plug
- 5 Transmitter

PROFINET: MRP (Media Redundancy Protocol)

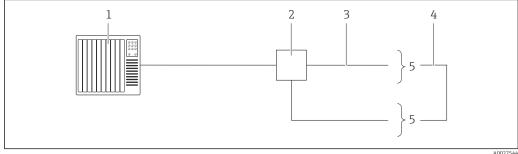


- Control system (e.g. PLC)
- 2 Ethernet switch
- 3
- Connecting cable between the two transmitters
- Transmitter

FOUNDATION Fieldbus

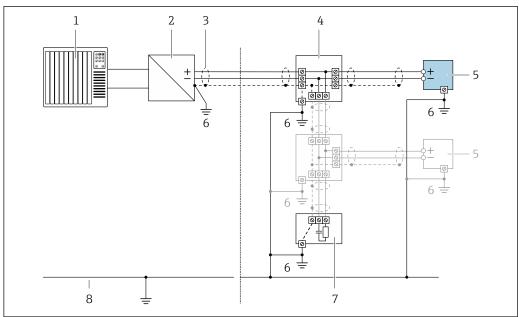

- **₽** 9 Connection example for FOUNDATION Fieldbus
- 1
- Control system (e.g. PLC) Power Conditioner (FOUNDATION Fieldbus)
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- T-box
- 5
- Measuring device Local grounding 6
- Bus terminator
- Potential matching line


Modbus RS485

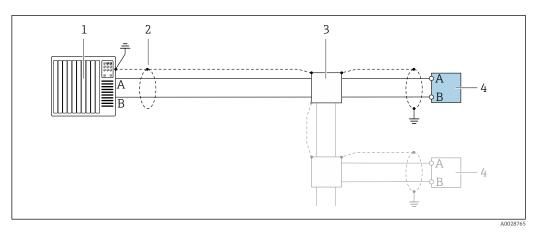

■ 10 Connection example for Modbus RS485, non-hazardous area and Zone 2; Class I, Division 2


- Control system (e.g. PLC)
- Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- Distribution box
- Transmitter

Current output 4-20 mA

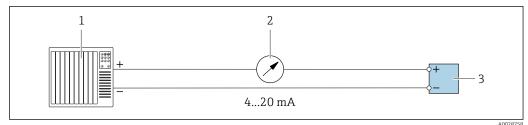

■ 11 Connection example for 4-20 mA current output (active)


- 1 Automation system with current input (e.g. PLC)
- 2 Analog display unit: observe maximum load
- 3 Transmitter

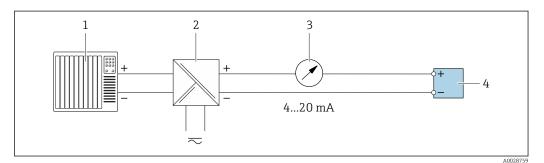

■ 12 Connection example for 4-20 mA current output (passive)

- 1 Automation system with current input (e.g. PLC)
- 2 Active barrier for power supply (e.g. RN221N)
- 3 Analog display unit: observe maximum load
- 4 Transmitter

Pulse/frequency output

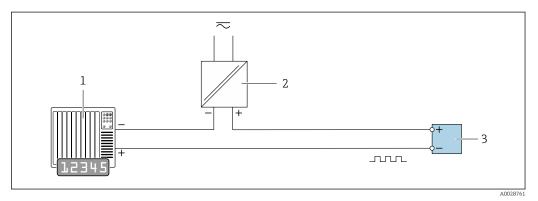


 \blacksquare 13 Connection example for pulse/frequency output (passive)

- 1 Automation system with pulse/frequency input (e.g. PLC)
- 2 Power supply

40 Endress+Hauser

1100207


Switch output

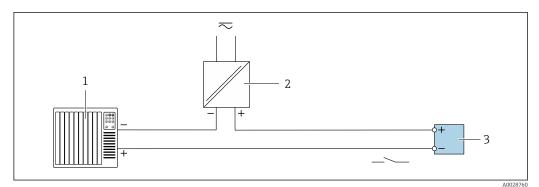


Connection example for switch output (passive)

- Automation system with switch input (e.g. PLC)
- Power supply
- *Transmitter: Observe input values* $\rightarrow \blacksquare 16$

Double pulse output

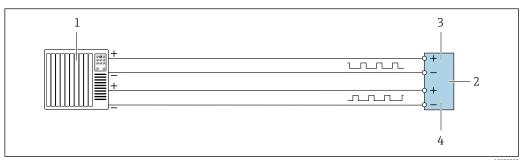


- **■** 15 Connection example for double pulse output (active)
- Automation system with double pulse input (e.g. PLC)
- 2
- 3 Double pulse output
- Double pulse output (slave), phase-shifted

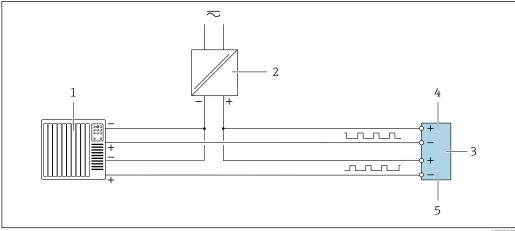

A0029279

- **■** 16 Connection example for double pulse output (passive)
- Automation system with double pulse input (e.g. PLC)
- 2 Power supply
- 3 *Transmitter: Observe input values* → 🖺 18
- Double pulse output
- Double pulse output (slave), phase-shifted


Relay output

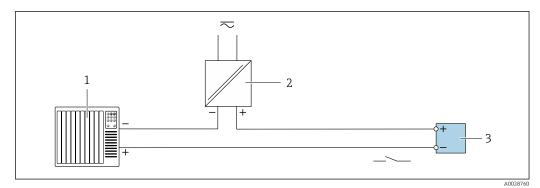

■ 17 Connection example for relay output (passive)

- 1 Automation system with relay input (e.g. PLC)
- 2 Power supply
- *3* Transmitter: Observe input values → 🖺 18


Current input

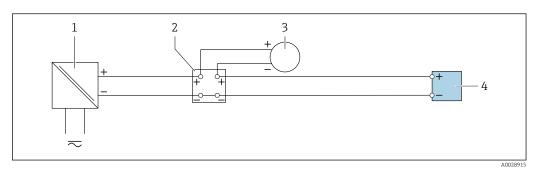

■ 18 Connection example for 4 to 20 mA current input

- 1 Power supply
- 2 Terminal box
- 3 External measuring device (for reading in pressure or temperature, for instance)
- 4 Transmitter

Status input

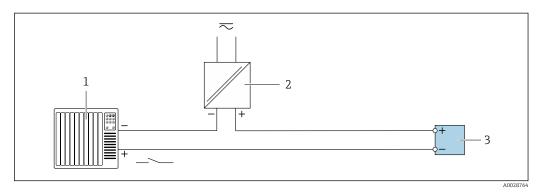

© 19 Connection example for status input

- 1 Automation system with status output (e.g. PLC)
- 2 Power supply
- 3 Transmitter

Potential equalization

Requirements

No special measures for potential equalization are required.

42

Please consider the following to ensure correct measurement:

- Same electrical potential for the fluid and sensor
- Company-internal grounding concepts

terminals

Spring-loaded terminals: Suitable for strands and strands with ferrules. Conductor cross-section 0.2 to 2.5 mm 2 (24 to 12 AWG).

Cable entries

- Cable gland: M20 \times 1.5 with cable Ø 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
 - NPT ½"
 - G ½"
 - M20
- Device plug for connecting cable: M12
 A device plug is always used for the device version with the order code for "Sensor connection housing", option C "Ultra-compact, hygienic, stainless".

Cable specification

Permitted temperature range

- The installation guidelines that apply in the country of installation must be observed.
- The cables must be suitable for the minimum and maximum temperatures to be expected.

Power supply cable

Standard installation cable is sufficient.

Protective ground cable

Cable $\geq 2.08 \text{ mm}^2 \text{ (14 AWG)}$

The grounding impedance must be less than 1 Ω .

Signal cable

Current output 4 to 20 mA HART

A shielded cable is recommended. Observe grounding concept of the plant.

PROFIBUS PA

Twisted, shielded two-wire cable. Cable type A is recommended .



For further information on planning and installing PROFIBUS networks see:

- Operating Instructions "PROFIBUS DP/PA: Guidelines for planning and commissioning" (BA00034S)
- PNO Directive 2.092 "PROFIBUS PA User and Installation Guideline"
- IEC 61158-2 (MBP)

PROFIBUS DP

The IEC 61158 standard specifies two types of cable (A and B) for the bus line which can be used for every transmission rate. Cable type A is recommended.

| Cable type | A | | | |
|---|---------------------------------|--|--|--|
| Characteristic impedance 135 to 165 Ω at a measuring frequency of 3 to 20 MHz | | | | |
| Cable capacitance | < 30 pF/m | | | |
| Wire cross-section | > 0.34 mm ² (22 AWG) | | | |
| Cable type | Twisted pairs | | | |
| Loop resistance | ≤110 Ω/km | | | |

| Signal damping | Max. 9 dB over the entire length of the cable cross-section | | | |
|----------------|--|--|--|--|
| Shield | Copper braided shielding or braided shielding with foil shield. When grounding the cable shield, observe the grounding concept of the plant. | | | |



For further information on planning and installing PROFIBUS networks see:

- Operating Instructions "PROFIBUS DP/PA: Guidelines for planning and commissioning" (BA00034S)
- PNO Directive 2.092 "PROFIBUS PA User and Installation Guideline"
- IEC 61158-2 (MBP)

EtherNet/IP

The standard ANSI/TIA/EIA-568-B.2 Annex specifies CAT 5 as the minimum category for a cable used for EtherNet/IP. CAT 5e and CAT 6 are recommended.



For more information on planning and installing EtherNet/IP networks, please refer to the "Media Planning and Installation Manual. EtherNet/IP" of ODVA Organization

PROFINET

Standard IEC 61156-6 specifies CAT 5 as the minimum category for a cable used for PROFINET. CAT 5e and CAT 6 are recommended.



For more information on planning and installing PROFINET networks, see: "PROFINET Cabling and Interconnection Technology" (2011) in a Cartesian Technology (2011) in and Interconnection Technology", Guideline for PROFINET

FOUNDATION Fieldbus

Twisted, shielded two-wire cable.



For further information on planning and installing FOUNDATION Fieldbus networks see:

- Operating Instructions for "FOUNDATION Fieldbus Overview" (BA00013S)
- FOUNDATION Fieldbus Guideline
- IEC 61158-2 (MBP)

Modbus RS485

The EIA/TIA-485 standard specifies two types of cable (A and B) for the bus line which can be used for every transmission rate. Cable type A is recommended.

| Cable type | A | | | |
|---|--|--|--|--|
| Characteristic impedance 135 to 165 Ω at a measuring frequency of 3 to 20 MHz | | | | |
| Cable capacitance | < 30 pF/m | | | |
| Wire cross-section | > 0.34 mm² (22 AWG) | | | |
| Cable type | Twisted pairs | | | |
| Loop resistance | ≤110 Ω/km | | | |
| Signal damping | Max. 9 dB over the entire length of the cable cross-section | | | |
| Shield | Copper braided shielding or braided shielding with foil shield. When grounding the cable shield, observe the grounding concept of the plant. | | | |

Current output 0/4 to 20 mA

Standard installation cable is sufficient.

Pulse/frequency/switch output

Standard installation cable is sufficient.

Double pulse output

Standard installation cable is sufficient.

Relay output

Standard installation cable is sufficient.

Current input 0/4 to 20 mA


Standard installation cable is sufficient.

Status input

Standard installation cable is sufficient.

Choice of connecting cable between the transmitter and sensor

Depends on the type of transmitter and the installation zones

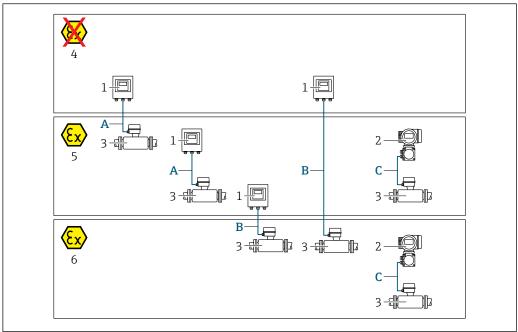

A0032476

- 1 Proline 500 digital transmitter
- 2 Proline 500 transmitter
- 3 Sensor Promass
- 4 Non-hazardous area
- 5 Hazardous area: Zone 2; Class I, Division 2
- 6 Hazardous area: Zone 1; Class I, Division 1
- A Standard cable to 500 digital transmitter → 🖺 45

 Transmitter installed in the non-hazardous area or hazardous area: Zone 2; Class I, Division 2 / sensor installed in the hazardous area: Zone 2; Class I, Division 2
- B Standard cable to 500 digital transmitter →

 46

 Transmitter installed in the hazardous area: Zone 2; Class I, Division 2 / sensor installed in the hazardous area: Zone 1; Class I, Division 1
- C Signal cable to 500 transmitter → 🖺 48

 Transmitter and sensor installed in the hazardous area: Zone 2; Class I, Division 2 oder Zone 1;

 Class I, Division 1

A: Connecting cable between sensor and transmitter: Proline 500 – digital

Standard cable

A standard cable with the following specifications can be used as the connecting cable.

| Design | 4 cores (2 pairs); uninsulated stranded CU wires; pair-stranded with common shield | | | |
|-----------------|--|--|--|--|
| Shielding | Tin-plated copper-braid, optical cover ≥ 85 % | | | |
| Loop resistance | Power supply line (+, –): maximum $10~\Omega$ | | | |
| Cable length | Maximum 300 m (1000 ft), see the following table. | | | |

| Cross-section | Cable length [max.] |
|-------------------------------|---------------------|
| 0.34 mm ² (AWG 22) | 80 m (270 ft) |
| 0.50 mm ² (AWG 20) | 120 m (400 ft) |
| 0.75 mm ² (AWG 18) | 180 m (600 ft) |
| 1.00 mm ² (AWG 17) | 240 m (800 ft) |
| 1.50 mm ² (AWG 15) | 300 m (1000 ft) |

Optionally available connecting cable

| Design | $2 \times 2 \times 0.34~\text{mm}^2$ (AWG 22) PVC cable $^{1)}$ with common shield (2 pairs, uninsulated stranded CU wires; pair-stranded) | | | |
|------------------------|--|--|--|--|
| Flame resistance | According to DIN EN 60332-1-2 | | | |
| Oil-resistance | According to DIN EN 60811-2-1 | | | |
| Shielding | Tin-plated copper-braid, optical cover \geq 85 % | | | |
| Operating temperature | When mounted in a fixed position: -50 to $+105$ °C (-58 to $+221$ °F); when cable can move freely: -25 to $+105$ °C (-13 to $+221$ °F) | | | |
| Available cable length | Fixed: 20 m (65 ft); variable: up to maximum 50 m (165 ft) | | | |


1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

B: Connecting cable between sensor and transmitter: Proline 500 - digital

Standard cable

A standard cable with the following specifications can be used as the connecting cable.

| Design | 4, 6, 8 cores (2, 3, 4 pairs); uninsulated stranded CU wires; pair-stranded with common shield | | | |
|-----------------------------------|--|--|--|--|
| Shielding | Tin-plated copper-braid, optical cover ≥ 85 % | | | |
| Capacitance C | Maximum 760 nF IIC, maximum 4.2 μF IIB | | | |
| Inductance L | Maximum 26 μH IIC, maximum 104 μH IIB | | | |
| Inductance/resistance ratio (L/R) | Maximum 8.9 $\mu H/\Omega$ IIC, maximum 35.6 $\mu H/\Omega$ IIB (e.g. in accordance with IEC 60079-25) | | | |
| Loop resistance | Power supply line (+, –): maximum 5 Ω | | | |
| Cable length | Maximum 150 m (500 ft), see the following table. | | | |

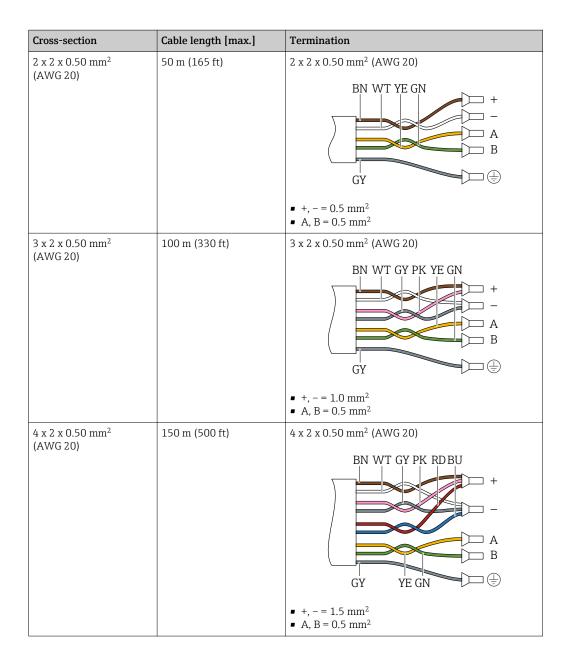

Optionally available connecting cable

| Connecting cable for | Zone 1; Class I, Division 1 | | |
|------------------------|--|--|--|
| Standard cable | $2 \times 2 \times 0.5 \text{ mm}^2$ (AWG 20) PVC cable $^{1)}$ with common shield (2 pairs, pairstranded) | | |
| Flame resistance | According to DIN EN 60332-1-2 | | |
| Oil-resistance | According to DIN EN 60811-2-1 | | |
| Shielding | Tin-plated copper-braid, optical cover \geq 85 % | | |
| Operating temperature | When mounted in a fixed position: -50 to $+105$ °C (-58 to $+221$ °F); when cable can move freely: -25 to $+105$ °C (-13 to $+221$ °F) | | |
| Available cable length | Fixed: 20 m (65 ft); variable: up to maximum 50 m (165 ft) | | |

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

C: Connecting cable between sensor and transmitter: Proline 500

| Standard cable | $6\times0.38\ mm^2$ PVC cable $^{1)}$ with common shield and individually shielded cores | | |
|-------------------------------------|--|--|--|
| Conductor resistance | ≤50 Ω/km (0.015 Ω/ft) | | |
| Capacitance: core/shield | <420 pF/m (128 pF/ft) | | |
| Cable length (max.) | 20 m (65 ft) | | |
| Cable lengths (available for order) | 5 m (15 ft), 10 m (32 ft), 20 m (65 ft) | | |
| Operating temperature | max. 105 °C (221 °F) | | |

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

Performance characteristics

Reference operating conditions

- Error limits based on ISO 11631
- Water with +15 to +45 °C (+59 to +113 °F) at2 to 6 bar (29 to 87 psi)
- Specifications as per calibration protocol
- Accuracy based on accredited calibration rigs that are traced to ISO 17025.
- i

To obtain measured errors, use the *Applicator* sizing tool $\rightarrow \implies 100$

Maximum measured error

o.r. = of reading; $1 \text{ g/cm}^3 = 1 \text{ kg/l}$; T = medium temperature

Base accuracy



Design fundamentals $\rightarrow \implies 51$

Mass flow and volume flow (liquids)

±0.10 % o.r.

Mass flow (gases)

±0.50 % o.r. (tantalum)

Density (liquids)

| Under reference operating conditions | Standard density calibration ¹⁾ | Wide-range Density specification ^{2) 3)} | | |
|--------------------------------------|---|--|--|--|
| [g/cm³] | [g/cm³] | [g/cm³] | | |
| ±0.0005 | ±0.02 | ±0.002 | | |

- 1) Valid over the entire temperature and density range
- Valid range for special density calibration: 0 to 2 g/cm³, +10 to +80 °C (+50 to +176 °F)
- 3) Order code for "Application package", option EE "Special density"

Temperature

 $\pm 0.5~^{\circ}\text{C} \pm 0.005 \cdot \text{T}~^{\circ}\text{C} \; (\pm 0.9~^{\circ}\text{F} \pm 0.003 \cdot (\text{T} - 32)~^{\circ}\text{F})$

Zero point stability

| DN | | Zero point stability | | |
|------|------|----------------------|----------|--|
| [mm] | [in] | [kg/h] | [lb/min] | |
| 8 | 3/8 | 0.40 | 0.015 | |
| 15 | 1/2 | ½ 0.65 0.02· | | |
| 25 | 1 | 1.80 0.066 | | |
| 40 | 1½ | 9.00 | 0.331 | |
| 50 | 2 | 14.00 | 0.514 | |

Flow values

Flow values as turndown parameter depending on nominal diameter. \\

SI units

| DN | 1:1 | 1:10 | 1:20 | 1:50 | 1:100 | 1:500 |
|------|--------|--------|--------|--------|--------|--------|
| [mm] | [kg/h] | [kg/h] | [kg/h] | [kg/h] | [kg/h] | [kg/h] |
| 8 | 2 000 | 200 | 100 | 40 | 20 | 4 |
| 15 | 6 500 | 650 | 325 | 130 | 65 | 13 |
| 25 | 18 000 | 1800 | 900 | 360 | 180 | 36 |
| 40 | 45 000 | 4500 | 2 250 | 900 | 450 | 90 |
| 50 | 70 000 | 7 000 | 3 500 | 1400 | 700 | 140 |

US units

| DN | 1:1 | 1:10 | 1:20 | 1:50 | 1:100 | 1:500 |
|--------|----------|----------|----------|----------|----------|----------|
| [inch] | [lb/min] | [lb/min] | [lb/min] | [lb/min] | [lb/min] | [lb/min] |
| 3/8 | 73.50 | 7.350 | 3.675 | 1.470 | 0.735 | 0.147 |
| 1/2 | 238.9 | 23.89 | 11.95 | 4.778 | 2.389 | 0.478 |
| 1 | 661.5 | 66.15 | 33.08 | 13.23 | 6.615 | 1.323 |
| 11/2 | 1654 | 165.4 | 82.70 | 33.08 | 16.54 | 3.308 |
| 2 | 2 5 7 3 | 257.3 | 128.7 | 51.46 | 25.73 | 5.146 |

Accuracy of outputs

The outputs have the following base accuracy specifications.

Current output

| Accuracy ±5 μA | |
|----------------|--|
|----------------|--|

Pulse/frequency output

o.r. = of reading

| Accuracy | Max. ±50 ppm o.r. (over the entire ambient temperature range) |
|----------|---|
|----------|---|

Repeatability

o.r. = of reading; $1 \text{ g/cm}^3 = 1 \text{ kg/l}$; T = medium temperature

Base repeatability



Design fundamentals $\rightarrow \implies 51$

Mass flow and volume flow (liquids)

±0.05 % o.r.

Mass flow (gases)

±0.25 % o.r. (tantalum)

Density (liquids)

 $\pm 0.00025 \text{ g/cm}^3$

Temperature

 $\pm 0.25 \text{ }^{\circ}\text{C} \pm 0.0025 \cdot \text{T} \text{ }^{\circ}\text{C} \ (\pm 0.45 \text{ }^{\circ}\text{F} \pm 0.0015 \cdot (\text{T}-32) \text{ }^{\circ}\text{F})$

Response time

The response time depends on the configuration (damping).

Influence of ambient temperature

Current output

| Temperature coefficient | Max. 1 μΑ/°C |
|-------------------------|--------------|
|-------------------------|--------------|

Pulse/frequency output

| Temperature coefficient | No additional effect. Included in accuracy. |
|-------------------------|---|
|-------------------------|---|

Influence of medium temperature

Mass flow and volume flow

o.f.s. = of full scale value

When there is a difference between the temperature for zero point adjustment and the process temperature, the additional measured error of the sensor is typically ± 0.0002 % o.f.s./°C (± 0.0001 % o.f.s./°F).


The effect is reduced if zero point adjustment is performed at process temperature.

Density

When there is a difference between the density calibration temperature and the process temperature, the typical measured error of the sensor is ± 0.0001 g/cm³ /°C (± 0.00005 g/cm³ /°F). Field density calibration is possible.

Wide-range density specification (special density calibration)

If the process temperature is outside the valid range (\Rightarrow \triangleq 48) the measured error is ± 0.0001 g/cm³ /°C (± 0.00005 g/cm³ /°F)

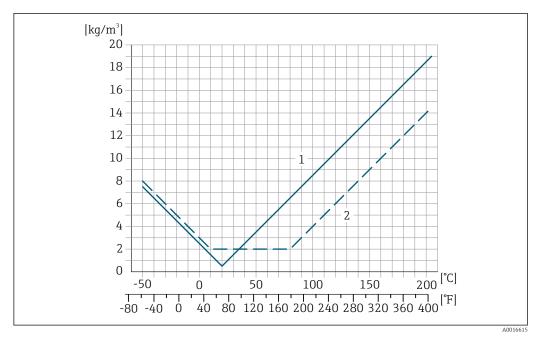

- Field density calibration, for example at $+20 \,^{\circ}\text{C}$ (+68 $^{\circ}\text{F}$)
- Special density calibration

Temperature

 $\pm 0.005 \cdot \text{T} \,^{\circ}\text{C} \, (\pm 0.005 \cdot (\text{T} - 32) \,^{\circ}\text{F})$

Influence of medium pressure

The table below shows the effect on accuracy of mass flow due to a difference between calibration pressure and process pressure.

o.r. = of reading



It is possible to compensate for the effect by:

- Reading in the current pressure measured value via the current input.
- Specifying a fixed value for the pressure in the device parameters.



Operating Instructions \rightarrow \blacksquare 101.

| DN | | Promass H zirconium | 702/R 60702 | Promass H tantalum 2.5W | |
|------|------|---------------------|--------------|-------------------------|--------------|
| [mm] | [in] | [% o.r./bar] | [% o.r./psi] | [% o.r./bar] | [% o.r./psi] |
| 8 | 3/8 | -0.017 | -0.0012 | -0.007 | -0.0005 |
| 15 | 1/2 | -0.021 | -0.0014 | -0.005 | -0.0003 |
| 25 | 1 | -0.013 | -0.0009 | -0.015 | -0.0010 |
| 40 | 1½ | -0.018 | -0.0012 | -0.012 | -0.0008 |
| 50 | 2 | -0.015 | -0.0010 | -0.011 | -0.0008 |

Design fundamentals

o.r. = of reading, o.f.s. = of full scale value

BaseAccu = base accuracy in % o.r., BaseRepeat = base repeatability in % o.r.

MeasValue = measured value; ZeroPoint = zero point stability


Calculation of the maximum measured error as a function of the flow rate

| Flow rate | | Maximum measured error in % o.r. |
|---|----------|----------------------------------|
| $\geq \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ | | ± BaseAccu |
| | A0021332 | ROULISS |
| $< \frac{\text{ZeroPoint}}{\text{BaseAccu}} \cdot 100$ | | ± ZeroPoint MeasValue · 100 |
| | A0021333 | A0021334 |

Calculation of the maximum repeatability as a function of the flow rate

| Flow rate | Maximum repeatability in % o.r. |
|---|---|
| $\geq \frac{\frac{1}{2} \cdot ZeroPoint}{BaseRepeat} \cdot 100$ | ± BaseRepeat |
| A0021335 | 1002270 |
| $<\frac{\frac{1}{2} \cdot ZeroPoint}{BaseRepeat} \cdot 100$ | $\pm \frac{1}{2} \cdot \frac{\text{ZeroPoint}}{\text{MeasValue}} \cdot 100$ |
| A0021336 | A0021337 |

Example for maximum measured error

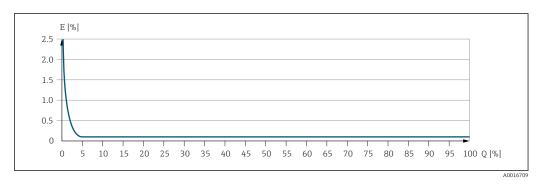


- Е Maximum measured error in % o.r. (example)
- Flow rate in % of maximum full scale value

Installation

No special measures such as supports etc. are necessary. External forces are absorbed by the construction of the device.

Mounting location

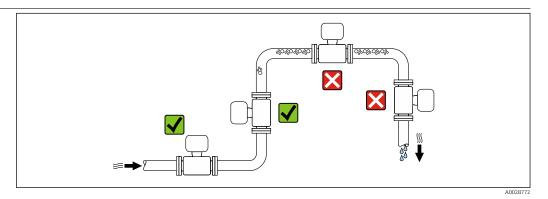


To prevent measuring errors arising from accumulation of gas bubbles in the measuring tube, avoid the following mounting locations in the pipe:

- Highest point of a pipeline.
- Directly upstream of a free pipe outlet in a down pipe.

Installation in down pipes

However, the following installation suggestion allows for installation in an open vertical pipeline. Pipe restrictions or the use of an orifice with a smaller cross-section than the nominal diameter prevent the sensor running empty while measurement is in progress.

52

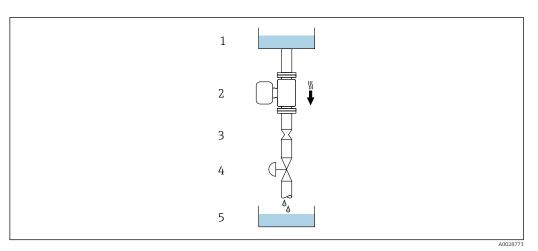

■ 20 Installation in a down pipe (e.g. for batching applications)

- 1 Supply tank
- 2 Sensor
- 3 Orifice plate, pipe restriction
- 4 Valve
- 5 Batching tank

| D | N | Ø orifice plate, pipe restriction | | |
|------|------|-----------------------------------|------|--|
| [mm] | [in] | [mm] | [in] | |
| 8 | 3/8 | 6 | 0.24 | |
| 15 | 1/2 | 10 | 0.40 | |
| 25 | 1 | 14 | 0.55 | |
| 40 | 11/2 | 22 | 0.87 | |
| 50 | 2 | 28 | 1.10 | |


Orientation

The direction of the arrow on the sensor nameplate helps you to install the sensor according to the flow direction (direction of medium flow through the piping).

| | Orientation | | | |
|---|---|----------|--|--|
| A | Vertical orientation | A0015591 | √ √ ¹⁾ | |
| В | Horizontal orientation, transmitter at top | A0015589 | | |
| С | Horizontal orientation, transmitter at bottom | A0015590 | Exceptions: $\rightarrow \ \square \ 21, \ \square \ 54$ | |
| D | Horizontal orientation, transmitter at side | A0015592 | | |

- 1) This orientation is recommended to ensure self-draining.
- 2) Applications with low process temperatures may decrease the ambient temperature. To maintain the minimum ambient temperature for the transmitter, this orientation is recommended.
- 3) Applications with high process temperatures may increase the ambient temperature. To maintain the maximum ambient temperature for the transmitter, this orientation is recommended.

If a sensor is installed horizontally with a curved measuring tube, match the position of the sensor to the fluid properties.

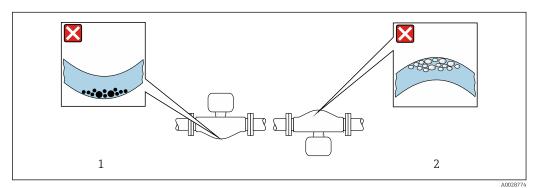

eals 21 Orientation of sensor with curved measuring tube


- 1 Avoid this orientation for fluids with entrained solids: Risk of solids accumulating.
- 2 Avoid this orientation for outgassing fluids: Risk of gas accumulating.

Inlet and outlet runs

Mounting the transmitter housing


Proline 500 - digital transmitter

Post mounting

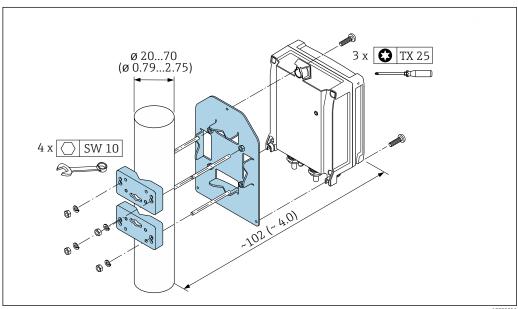

■ 22 Engineering unit mm (in)

Wall mounting

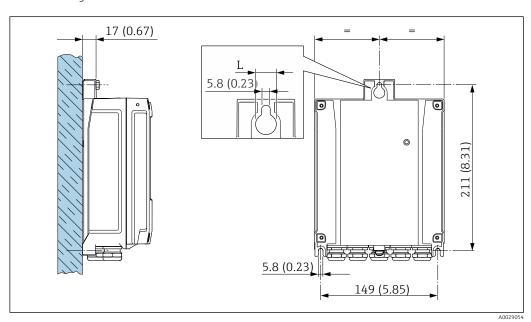

■ 23 Engineering unit mm (in)

L Depends on order code for "Transmitter housing"

Order code for "Transmitter housing"

- Option **A**, aluminum coated: L = 14 mm (0.55 in)
- Option **D**, polycarbonate: L = 13 mm (0.51 in)

Endress+Hauser 55

A002905

Proline 500 transmitter


Post mounting

A WARNING

Order code for "Transmitter housing", option L "Cast, stainless": cast transmitters are very heavy.


They are unstable if they are not mounted on a secure, fixed post.

▶ Only mount the transmitter on a secure, fixed post on a stable surface.

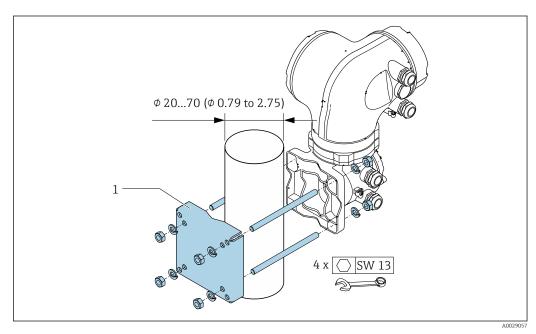

■ 24 Engineering unit mm (in)

Wall mounting

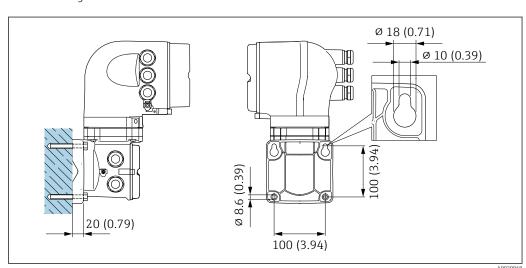

■ 25 Engineering unit mm (in)

Special mounting instructions

Drainability


The measuring tubes can be completely drained and protected against solids build-up in vertical orientation.

Zero point adjustment


Experience shows that zero point adjustment is advisable only in special cases:

- To achieve maximum measuring accuracy even with low flow rates.
- Under extreme process or operating conditions (e.g. very high process temperatures or very highviscosity fluids).

Protective cover

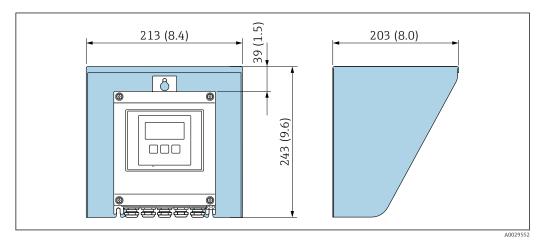

■ 26 Weather protection cover for Proline 500 – digital

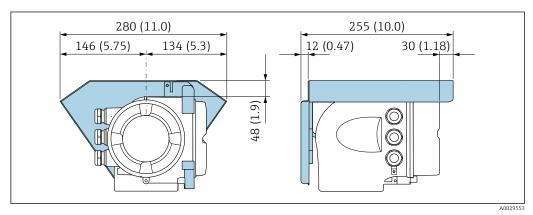

■ 27 Weather protection cover for Proline 500

Environment

Ambient temperature range

| Measuring device | -40 to +60 °C (-40 to +140 °F) Order code for "Test, certificate", option JP: -50 to +60 °C (-58 to +140 °F) |
|----------------------------------|--|
| Readability of the local display | -20 to +60 °C (-4 to +140 °F) The readability of the display may be impaired at temperatures outside the temperature range. |

Dependency of ambient temperature on medium temperature $\rightarrow \implies 58$

► If operating outdoors: Avoid direct sunlight, particularly in warm climatic regions.

| Storage temperature | –50 to +80 °C (−58 to +176 °F) |
|---|--|
| Climate class | DIN EN 60068-2-38 (test Z/AD) |
| Degree of protection | Transmitter ■ As standard: IP66/67, type 4X enclosure ■ When housing is open: IP20, type 1 enclosure ■ Display module: IP20, type 1 enclosure |
| | Sensor ■ As standard: IP66/67, type 4X enclosure ■ With the order code for "Sensor options", option CM : IP69 can also be ordered |
| | External WLAN antenna IP67 |
| Vibration resistance | Oscillation, sinusoidal, following IEC 60068-2-6 2 to 8.4 Hz, 3.5 mm peak Oscillation, broadband noise following IEC 60068-2-64 10 to 200 Hz, 0.003 g²/Hz 200 to 2000 Hz, 0.001 g²/Hz Total: 1.54 g rms |
| Shock resistance Shock, half-sine according to IEC 60068-2-27 6 ms 50 g | |
| Shock resistance | Shock due to rough handling following IEC 60068-2-31 |
| Interior cleaning | Cleaning in place (CIP)Sterilization in place (SIP) |
| | Options Oil- and grease-free version for wetted parts, without declaration Order code for "Service", option HA |
| Electromagnetic compatibility (EMC) | As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21) Device version with PROFIBUS DP: Complies with emission limits for industry as per EN 50170 |

Details are provided in the Declaration of Conformity.

Process

Volume 2, IEC 61784

Medium temperature range


| -50 to $+205$ °C (-58 to $+401$ °F) for zirconium 702 /R 60702 | Order code for "Measuring tube mat., wetted surface", option DA |
|---|---|
| -50 to $+150$ °C (-58 to $+302$ °F) for tantalum 2.5 W | Order code for "Measuring tube mat., wetted surface", option EA |

The following applies for PROFIBUS DP: If baud rates > 1.5 MBaud, an EMC cable entry must be

used and the cable shield must continue as far as the terminal wherever possible.

58

Dependency of ambient temperature on medium temperature

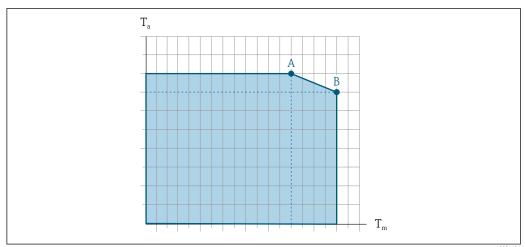

- 28 Exemplary representation, values in the table below.
- *T_a* Ambient temperature
- T_m Medium temperature
- A Maximum permitted medium temperature T_m at $T_{a max}$ = 60 °C (140 °F); higher medium temperatures T_m require a reduced ambient temperature T_a
- B Maximum permitted ambient temperature T_a for the maximum specified medium temperature T_m of the sensor
- Values for devices used in the hazardous area: Separate Ex documentation (XA) for the device $\rightarrow \triangleq 102$.

| | Not insulated | | | | Insulated | | | | | |
|---|----------------|-----------------|----|----------------|----------------|-----------------|--------------|-----------------|--|--|
| | A | | | | A | | В | | | |
| Version 1) | Ta | T_{m} | Ta | T _m | Ta | T_{m} | Ta | T_{m} | | |
| Tantalum (order code for "Measuring tube mat.", option EA) | 60 °C (140 °F) | 150 °C (302 °F) | - | - | 60 °C (140 °F) | 150 °C (302 °F) | - | - | | |
| Zirconium 702 (order code for "Measuring tube mat.", option DA) | 60 °C (140 °F) | 205 °C (401 °F) | - | - | 60 °C (140 °F) | 150 °C (302 °F) | 55 ℃ (131 ℉) | 205 °C (401 °F) | | |


1) The values apply for Promass H 500 - digital and Promass H 500.

Density 0 to $5\,000\,\text{kg/m}^3$ (0 to $3\,12\,\text{lb/cf}$)

Pressure-temperature ratings

The following pressure/temperature diagrams apply to all pressure-bearing parts of the device and not just the process connection. The diagrams show the maximum permissible medium pressure depending on the specific medium temperature.


Flange connection according to EN 1092-1 (DIN 2501)

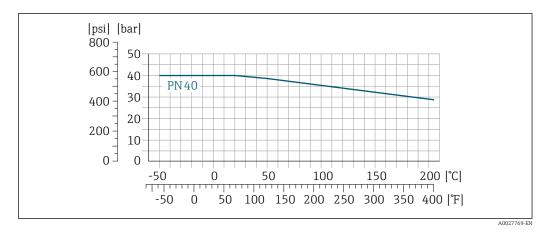

With flange material 1.4301 (304); wetted parts: zirconium 702, tantalum

The material load curves for the temperature range +150 to +205 °C (+302 to +401 °F) apply only to the order code for "Measuring tube material", option TJ


Flange connection according to ASME B16.5

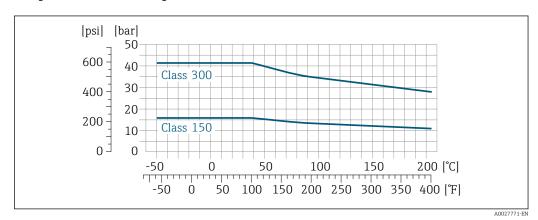

 \blacksquare 30 With flange material 1.4301 (304); wetted parts: zirconium 702, tantalum

The material load curves for the temperature range +150 to +205 °C (+302 to +401 °F) apply only to the order code for "Measuring tube material", option TJ

Flange connection according to JIS B2220

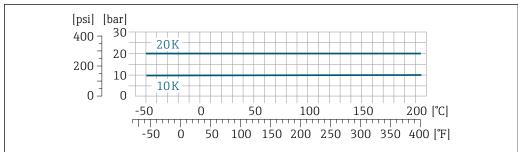

■ 31 With flange material 1.4301 (304); wetted parts: zirconium 702, tantalum

The material load curves for the temperature range +150 to +205 °C (+302 to +401 °F) apply only to the order code for "Measuring tube material", option TJ

Endress+Hauser

A0027772-EN

Sensor housing

The sensor housing is filled with dry nitrogen gas and protects the electronics and mechanics inside.

If a measuring tube fails (e.g. due to process characteristics like corrosive or abrasive fluids), the fluid will initially be contained by the sensor housing.

If the sensor is to be purged with gas (gas detection), it should be equipped with purge connections.

Do not open the purge connections unless the containment can be filled immediately with a dry, inert gas. Use only low pressure to purge. Maximum pressure: 5 bar (72.5 psi).

Sensor housing nominal pressure rating and burst pressure

The following sensor housing nominal pressure ratings/burst pressures are only valid for standard devices and/or devices equipped with closed purge connections (not opened/as delivered).

If a device fitted with purge connections (order code for "Sensor option", option CH "Purge connection") is connected to the purge system, the maximum nominal pressure is determined by the purge system itself or by the device, depending on which component has the lower nominal pressure classification.


The sensor housing burst pressure refers to a typical internal pressure which is reached prior to mechanical failure of the sensor housing and which was determined during type testing. The corresponding type test declaration can be ordered with the device (order code for "Additional approval", option LN "Sensor housing burst pressure, type test").

| D | N | pres | ing nominal sure a safety factor 4) | Sensor housing burst pressure | | |
|------|-------|-------|--|-------------------------------|---------|--|
| [mm] | [in] | [bar] | [psi] | [bar] | [psi] | |
| 8 | 8 3/8 | | 362 | 170 | 2 4 6 5 | |
| 15 | 1/2 | 25 | 362 | 160 | 2320 | |
| 25 | 1 | 25 | 362 | 130 | 1885 | |
| 40 | 1½ | 16 | 232 | 85 | 1232 | |
| 50 | 2 | 16 | 232 | 85 | 1232 | |

For information on the dimensions: see the "Mechanical construction" section → 🗎 63

Flow limit

Select the nominal diameter by optimizing between the required flow range and permissible pressure loss.



- The minimum recommended full scale value is approx. 1/20 of the maximum full scale value
- In most applications, 20 to 50 % of the maximum full scale value can be considered ideal
- A low full scale value must be selected for abrasive media (such as liquids with entrained solids): flow velocity < 1 m/s (< 3 ft/s).
- For gas measurement the following rules apply:
 - The flow velocity in the measuring tubes should not exceed half the sound velocity (0.5 Mach).
 - The maximum mass flow depends on the density of the gas: formula $ightarrow~ ilde{f B}~11$
- To calculate the flow limit, use the *Applicator* sizing tool $\rightarrow \implies 100$

Pressure loss




System pressure

It is important that cavitation does not occur, or that gases entrained in the liquids do not outgas. This is prevented by means of a sufficiently high system pressure.

For this reason, the following mounting locations are recommended:

- At the lowest point in a vertical pipe
- Downstream from pumps (no danger of vacuum)



A002877

Thermal insulation

In the case of some fluids, it is important to keep the heat radiated from the sensor to the transmitter to a low level. A wide range of materials can be used for the required insulation.


The following device versions are recommended for versions with thermal insulation: Version with extended neck:

Order code for "Measuring tube material", option DA or EA with an extended neck length of $105\ mm\ (4.13\ in)$.

NOTICE

Electronics overheating on account of thermal insulation!

- Recommended orientation: horizontal orientation, sensor connection housing pointing downwards.
- ▶ Do not insulate the sensor connection housing.
- Maximum permissible temperature at the lower end of the sensor connection housing: 80 °C (176 °F)
- ► Thermal insulation with extended neck free: We recommend that you do not insulate the extended neck in order to ensure optimum dissipation of heat.

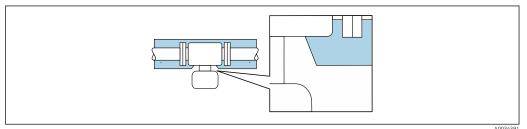

■ 32 Thermal insulation with extended neck free

Heating

Some fluids require suitable measures to avoid loss of heat at the sensor.

Heating options

- Electrical heating, e.g. with electric band heaters
- Via pipes carrying hot water or steam
- Via heating jackets



Heating jackets for the sensors can be ordered as accessories from Endress+Hauser . \rightarrow \bigcirc 99

NOTIC

Danger of overheating when heating

- ► Ensure that the temperature at the lower end of the transmitter housing does not exceed 80 °C (176 °F).
- ► Ensure that sufficient convection takes place at the transmitter neck.
- ► Ensure that a sufficiently large area of the transmitted neck remains exposed. The uncovered part serves as a radiator and protects the electronics from overheating and excessive cooling.
- ▶ If using in potentially explosive atmospheres, observe the information in the device-specific Ex documentation. For detailed information on the temperature tables, see the separate document entitled "Safety Instructions" (XA) for the device.

Vibrations

The high oscillation frequency of the measuring tubes ensures that the correct operation of the measuring system is not influenced by plant vibrations.


62

Mechanical construction

Dimensions in SI units

Housing of Proline 500 - digital transmitter

Non-hazardous area or hazardous area: Zone 2; Class I, Division 2

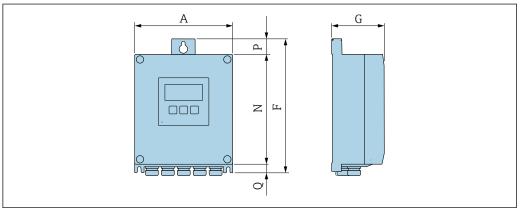

A0033789

Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"


| A | F | G | N | P | Q |
|------|------|------|------|------|------|
| [mm] | [mm] | [mm] | [mm] | [mm] | [mm] |
| 167 | 232 | 80 | 187 | 24 | |

 $\label{lem:code} \textit{Order code for "Transmitter housing", option D "Polycarbonate" and order code for "Integrated ISEM electronics", option A "Sensor"$

| A | F | G | N | P | Q |
|------|------|------|------|------|------|
| [mm] | [mm] | [mm] | [mm] | [mm] | [mm] |
| 177 | 234 | 90 | 197 | 17 | |

Housing of Proline 500 transmitter

Hazardous area: Zone 2; Class I, Division 2 or Zone 1; Class I, Division 1

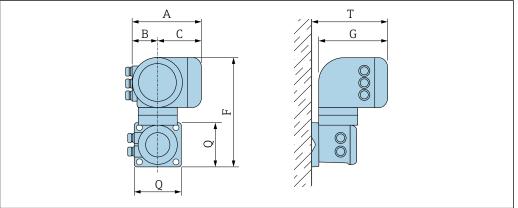

A0033788


Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option B "Transmitter"

| A | B | C | F | G | Q | T |
|------|------|------|------|------|------|------|
| [mm] |
| 188 | 85 | 103 | 318 | 217 | 130 | |

 $\label{lem:code_for_problem} \textit{Order code for "Transmitter housing", option L "Cast, stainless" and order code for "Integrated ISEM electronics", option B "Transmitter"$

| A | B | C | F | G | Q | T |
|------|------|------|------|------|------|------|
| [mm] |
| 188 | 85 | 103 | 295 | 217 | 130 | |

Sensor connection housing

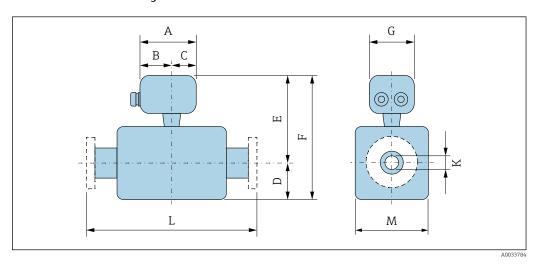

Order code for "Sensor connection housing", option A "Aluminum, coated"

| | , | | | 5, 1 | | <i>'</i> | | | | |
|------|------|------|------|------|------|----------|------|------|------|------|
| DN | A 1) | В | С | D | Е | F | G | K | L | М |
| [mm] | [mm] | [mm] | [mm] | [mm] |
| 8 | 148 | 94 | 54 | 108 | 261 | 369 | 136 | 5.35 | 2) | 92 |
| 15 | 148 | 94 | 54 | 108 | 261 | 369 | 136 | 8.30 | 2) | 92 |
| 25 | 148 | 94 | 54 | 121 | 261 | 382 | 136 | 12.0 | 2) | 92 |
| 40 | 148 | 94 | 54 | 173 | 285 | 458 | 136 | 17.6 | 2) | 132 |
| 50 | 148 | 94 | 54 | 241 | 296 | 537 | 136 | 26.0 | 2) | 167 |

- 1) Depending on the cable gland used: values up to \pm 30 mm
- 2) Dependent on the respective process connection

Order code for "Sensor connection housing", option B "Stainless"

| DN | A 1) | B 1) | С | D | E | F | G | K | L | М |
|------|------|------|------|------|------|------|------|------|------|------|
| [mm] |
| 8 | 137 | 78 | 59 | 108 | 257 | 365 | 134 | 5.35 | 2) | 92 |
| 15 | 137 | 78 | 59 | 108 | 257 | 365 | 134 | 8.30 | 2) | 92 |
| 25 | 137 | 78 | 59 | 121 | 257 | 378 | 134 | 12.0 | 2) | 92 |
| 40 | 137 | 78 | 59 | 173 | 281 | 454 | 134 | 17.6 | 2) | 132 |
| 50 | 137 | 78 | 59 | 241 | 292 | 533 | 134 | 26.0 | 2) | 167 |

- 1) Depending on the cable gland used: values up to + 30 mm
- 2) Dependent on the respective process connection

Order code for "Sensor connection housing", option C "Ultra-compact hygienic, stainless"

| DN | 1)A | 1)B | С | D | E | F | G | K | L | M |
|------|------|------|------|------|------|------|------|------|------|------|
| [mm] |
| 8 | 124 | 68 | 56 | 108 | 257 | 365 | 112 | 5.35 | 2) | 92 |
| 15 | 124 | 68 | 56 | 108 | 257 | 365 | 112 | 8.30 | 2) | 92 |
| 25 | 124 | 68 | 56 | 121 | 257 | 378 | 112 | 12.0 | 2) | 92 |
| 40 | 124 | 68 | 56 | 173 | 281 | 454 | 112 | 17.6 | 2) | 132 |
| 50 | 124 | 68 | 56 | 241 | 292 | 533 | 112 | 26.0 | 2) | 167 |

- 1) Depending on the cable gland used: values up to + 30 mm
- 2) Dependent on the respective process connection


Order code for "Sensor connection housing", option L "Cast, stainless"

| DN | A 1) | В | С | D | Е | F | G | K | L | M |
|------|------|------|------|------|------|------|------|------|------|------|
| [mm] |
| 8 | 145 | 86 | 59 | 108 | 284 | 392 | 136 | 5.35 | 2) | 92 |
| 15 | 145 | 86 | 59 | 108 | 284 | 392 | 136 | 8.30 | 2) | 92 |
| 25 | 145 | 86 | 59 | 121 | 284 | 405 | 136 | 12.0 | 2) | 92 |
| 40 | 145 | 86 | 59 | 173 | 308 | 481 | 136 | 17.6 | 2) | 132 |
| 50 | 145 | 86 | 59 | 241 | 319 | 560 | 136 | 26.0 | 2) | 167 |

- 1) Depending on the cable gland used: values up to \pm 30 mm
- 2) Dependent on the respective process connection

Flange connections

Fixed flange EN 1092-1, ASME B16.5, JIS B2220

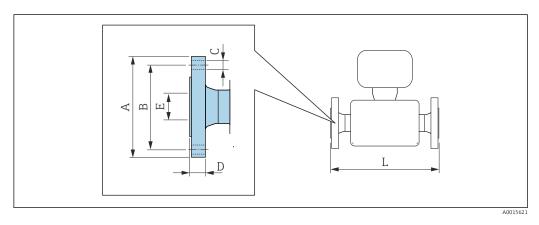

Length tolerance for dimension L in mm: +1.5 / -2.0

| 1.4404 (316/3 | Flange according to EN 1092-1 (DIN 2501): PN 40 1.4404 (316/316L) Order code for "Process connection", option D2W | | | | | | | | | | | |
|---|---|----|---------|----|------|-----|--|--|--|--|--|--|
| DN A B C D E L [mm] [mm] [mm] [mm] [mm] | | | | | | | | | | | | |
| 8 ¹⁾ | 95 | 65 | 4 × Ø14 | 20 | 17.3 | 336 | | | | | | |
| 15 95 65 4 × Ø14 20 17.3 440 | | | | | | | | | | | | |
| 25 115 85 4 × Ø14 19.0 28.5 580 | | | | | | | | | | | | |

| Flange according to EN 1092-1 (DIN 2501): PN 40 1.4404 (316/316L) Order code for "Process connection", option D2W | | | | | | | | | |
|---|--|-----|---------|------|------|------|--|--|--|
| DN A B C D E L [mm] [mm] [mm] [mm] [mm] | | | | | | | | | |
| 40 | 150 | 110 | 4 × Ø18 | 21.5 | 43.1 | 794 | | | |
| 50 | 165 | 125 | 4 × Ø18 | 23.5 | 54.5 | 1071 | | | |
| Surface roughn | Surface roughness (flange): EN 1092-1 Form B1 (DIN 2526 Form C), Ra 3.2 to 12.5 µm | | | | | | | | |

1) DN 8 with DN 15 flanges as standard

| Flange according to ASME B16.5: Cl 150 1.4404 (316/316L) Order code for "Process connection", option AAW | | | | | | | | | | |
|--|-----------|-----------|-----------|-----------|-----------|-----------|--|--|--|--|
| DN [mm] | A [mm] | B [mm] | C [mm] | D [mm] | E [mm] | L [mm] | | | | |
| 8 ¹⁾ | 90 | 60.3 | 4 × Ø15.7 | 12.8 | 15.7 | 336 | | | | |
| 15 | 90 | 60.3 | 4 × Ø15.7 | 12.8 | 15.7 | 440 | | | | |
| 25 | 110 | 79.4 | 4 × Ø15.7 | 15.1 | 26.7 | 580 | | | | |
| 40 | 125 | 98.4 | 4 × Ø15.7 | 17.5 | 40.9 | 794 | | | | |
| 50 150 120.7 4 × Ø19.1 23.6 52.6 1071 | | | | | | | | | | |
| Surface roughness (flange): Ra 3.2 to 6.3 µm | | | | | | | | | | |

1) DN 8 with DN 15 flanges as standard

| Flange according to ASME B16.5: Cl 300 1.4404 (316/316L) Order code for "Process connection", option ABW | | | | | | | | | | |
|--|--|-----------|-----------|-----------|-----------|-----------|--|--|--|--|
| DN [mm] | A [mm] | B [mm] | C [mm] | D [mm] | E [mm] | L [mm] | | | | |
| 8 ¹⁾ | 95 | 66.7 | 4 × Ø15.7 | 14.2 | 15.7 | 336 | | | | |
| 15 | 95 | 66.7 | 4 × Ø15.7 | 14.2 | 15.7 | 440 | | | | |
| 25 | 125 | 88.9 | 4 × Ø19.1 | 17.5 | 26.7 | 580 | | | | |
| 40 | 155 | 114.3 | 4 × Ø22.3 | 20.6 | 40.9 | 794 | | | | |
| 50 165 127.0 8 × Ø19.1 23.6 52.6 1071 | | | | | | | | | | |
| Surface rough | Surface roughness (flange): Ra 3.2 to 6.3 µm | | | | | | | | | |

1) DN 8 with DN 15 flanges as standard


| Flange JIS B2220: 10K 1.4301 (304), wetted parts: titanium Order code for "Process connection", option NDW | | | | | | | | | |
|--|-----------|-----------|-----------|-----------|-----------|-----------|--|--|--|
| DN [mm] | A [mm] | B [mm] | C [mm] | D [mm] | E [mm] | L [mm] | | | |
| 50 | 155 | 120 | 4 × Ø19 | 18.5 | 50 | 1071 | | | |

| 1.4404 (316/ | Flange JIS B2220: 20K 1.4404 (316/316L) Order code for "Process connection", option NEW | | | | | | | | | | |
|---|---|-----|---------|----|----|-----|--|--|--|--|--|
| DN A B C D E L [mm] [mm] [mm] [mm] [mm] | | | | | | | | | | | |
| 8 ¹⁾ | 95 | 70 | 4 × Ø15 | 14 | 15 | 336 | | | | | |
| 15 | 95 | 70 | 4 × Ø15 | 14 | 15 | 440 | | | | | |
| 25 | 125 | 90 | 4 × Ø19 | 16 | 25 | 580 | | | | | |
| 40 | 140 | 105 | 4 × Ø19 | 18 | 40 | 794 | | | | | |
| 50 165 120 8 × Ø19 22 50 1071 | | | | | | | | | | | |
| Surface roughr | Surface roughness (flange): Ra 3.2 to 6.3 µm | | | | | | | | | | |

DN 8 with DN 15 flanges as standard 1)

Accessories


Rinse connections

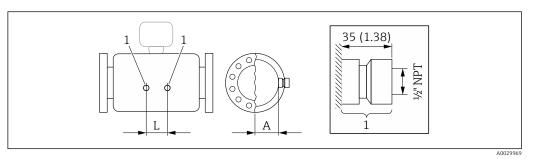


 $Connection\ nipple\ for\ purge\ connections: order\ code\ for\ "Sensor\ options",\ option\ CH\ "Purge\ connection"$

| DN | A | L | | |
|------|------|------|--|--|
| [mm] | [mm] | [mm] | | |
| 8 | 47 | 110 | | |
| 15 | 47 | 204 | | |
| 25 | 47 | 348 | | |
| 40 | 67 | 526 | | |
| 50 | 84.5 | 763 | | |

Protective cover

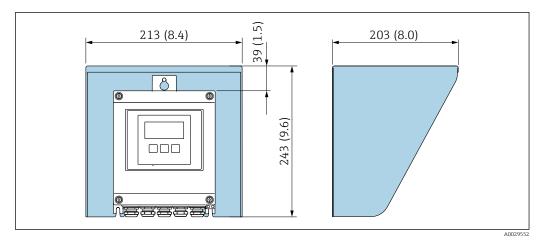

Weather protection cover for Proline 500 – digital

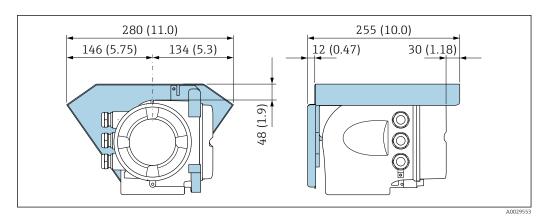


₹ 34 Weather protection cover for Proline 500

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

Proline 500 – digital


External WLAN antenna mounted on device

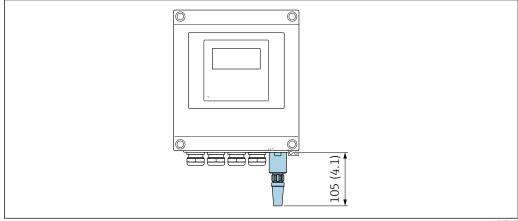

■ 35 Engineering unit mm (in)

External WLAN antenna mounted with cable


The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

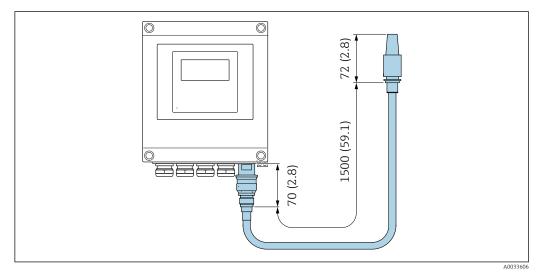

🖪 36 🛮 Engineering unit mm (in)

Proline 500


External WLAN antenna mounted on device

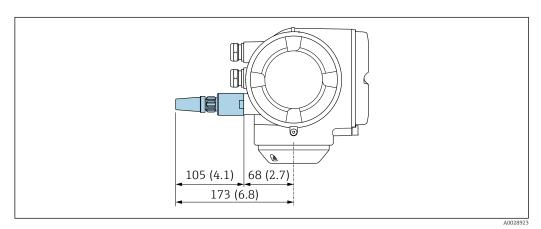

■ 37 Engineering unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

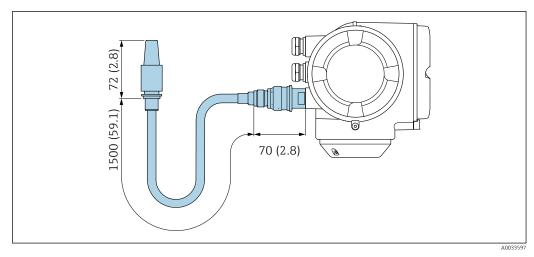


■ 38 Engineering unit mm (in)

Dimensions in US units

Housing of Proline 500 – digital transmitter

Non-hazardous area or hazardous area: Zone 2; Class I, Division 2

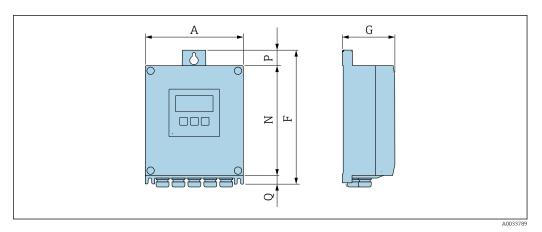

 $\label{lem:code} \textit{Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option A "Sensor"$

| A | F | G | N | P | Q |
|------|------|------|------|------|------|
| [in] | [in] | [in] | [in] | [in] | [in] |
| 6.57 | 9.13 | 3.15 | 7.36 | 0.94 | |


 $\label{lem:code} \textit{Order code for "Transmitter housing", option D "Polycarbonate" and order code for "Integrated ISEM electronics", option A "Sensor"$

| A | F | G | N | P | Q |
|------|------|------|------|------|------|
| [in] | [in] | [in] | [in] | [in] | [in] |
| 6.97 | 9.21 | 3.54 | 7.76 | 0.67 | |

Housing of Proline 500 transmitter

Hazardous area: Zone 2; Class I, Division 2 or Zone 1; Class I, Division 1

70

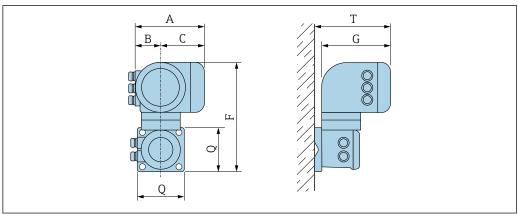

A003379


 $\label{lem:code_for_problem} \textit{Order code for "Transmitter housing", option A "Aluminum, coated" and order code for "Integrated ISEM electronics", option B "Transmitter"$

| A | B | C | F | G | Q | T |
|------|------|------|------|------|------|------|
| [in] |
| 7.40 | 3.35 | 4.06 | 12.5 | 8.54 | 5.12 | |

 $\label{lem:code} \textit{Order code for "Transmitter housing", option L "Cast, stainless" and order code for "Integrated ISEM electronics", option B "Transmitter"$

| A | B | C | F | G | Q | T |
|------|------|------|------|------|------|------|
| [in] |
| 7.40 | 3.35 | 4.06 | 11.6 | 8.54 | 5.12 | |

Sensor connection housing

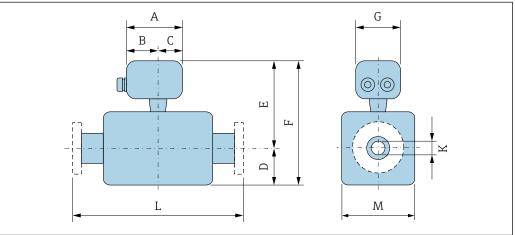

A0033784

Order code for "Sensor connection housing", option A "Aluminum, coated"

| DN | A 1) | В | С | D | Е | F | G | К | L | М |
|------|------|------|------|------|------|------|------|-------|------|------|
| [in] | [in] | [in] |
| 3/8 | 5.83 | 3.70 | 2.13 | 4.25 | 10.3 | 14.5 | 5.35 | 0.211 | 2) | 3.62 |
| 1/2 | 5.83 | 3.70 | 2.13 | 4.25 | 10.3 | 14.5 | 5.35 | 0.33 | 2) | 3.62 |
| 1 | 5.83 | 3.70 | 2.13 | 4.76 | 10.3 | 15.0 | 5.35 | 0.47 | 2) | 3.62 |

| DN | A 1) | В | С | D | E | F | G | K | L | М |
|------|------|------|------|------|------|------|------|------|------|------|
| [in] |
| 11/2 | 5.83 | 3.70 | 2.13 | 6.81 | 11.2 | 18.0 | 5.35 | 0.69 | 2) | 5.20 |
| 2 | 5.83 | 3.70 | 2.13 | 9.49 | 11.7 | 21.1 | 5.35 | 1.02 | 2) | 6.57 |

- 1) Depending on the cable gland used: values up to +1.18 in
- 2) Dependent on the respective process connection

Order code for "Sensor connection housing", option B "Stainless"

| DN | A 1) | B 1) | С | D | E | F | G | K | L | М |
|------|------|------|------|------|------|------|------|-------|------|------|
| [in] | [in] | [in] |
| 3/8 | 5.39 | 3.07 | 2.32 | 4.25 | 10.1 | 14.4 | 5.28 | 0.211 | 2) | 3.62 |
| 1/2 | 5.39 | 3.07 | 2.32 | 4.25 | 10.1 | 14.4 | 5.28 | 0.33 | 2) | 3.62 |
| 1 | 5.39 | 3.07 | 2.32 | 4.76 | 10.1 | 14.9 | 5.28 | 0.47 | 2) | 3.62 |
| 1½ | 5.39 | 3.07 | 2.32 | 6.81 | 11.1 | 17.9 | 5.28 | 0.69 | 2) | 5.20 |
| 2 | 5.39 | 3.07 | 2.32 | 9.49 | 11.5 | 21.0 | 5.28 | 1.02 | 2) | 6.57 |

- 1) Depending on the cable gland used: values up to +1.18 in
- 2) Dependent on the respective process connection

Order code for "Sensor connection housing", option C "Ultra-compact hygienic, stainless"

| DN | A 1) | B 1) | С | D | E | F | G | K | L | М |
|------|------|------|------|------|------|------|------|------|------|------|
| [in] |
| 3/8 | 4.88 | 2.68 | 2.20 | 4.25 | 10.1 | 14.4 | 4.41 | 0.21 | 2) | 3.62 |
| 1/2 | 4.88 | 2.68 | 2.20 | 4.25 | 10.1 | 14.4 | 4.41 | 0.33 | 2) | 3.62 |
| 1 | 4.88 | 2.68 | 2.20 | 4.76 | 10.1 | 14.9 | 4.41 | 0.47 | 2) | 3.62 |
| 1½ | 4.88 | 2.68 | 2.20 | 6.81 | 11.1 | 17.9 | 4.41 | 0.69 | 2) | 5.20 |
| 2 | 4.88 | 2.68 | 2.20 | 9.49 | 11.5 | 21.0 | 4.41 | 1.02 | 2) | 6.57 |

- 1) Depending on the cable gland used: values up to ± 1.18 in
- 2) Dependent on the respective process connection


Order code for "Sensor connection housing", option L "Cast, stainless"

| DN | A 1) | В | С | D | E | F | G | К | L | М |
|------|------|------|------|------|-------|-------|------|-------|------|------|
| [in] | [in] | [in] | [in] | [in] | [in] | [in] | [in] | [in] | [in] | [in] |
| 3/8 | 5.71 | 3.39 | 2.32 | 4.25 | 11.18 | 15.43 | 5.35 | 0.211 | 2) | 3.62 |
| 1/2 | 5.71 | 3.39 | 2.32 | 4.25 | 11.18 | 15.43 | 5.35 | 0.33 | 2) | 3.62 |
| 1 | 5.71 | 3.39 | 2.32 | 4.76 | 11.18 | 15.94 | 5.35 | 0.47 | 2) | 3.62 |
| 1½ | 5.71 | 3.39 | 2.32 | 6.81 | 12.13 | 18.94 | 5.35 | 0.69 | 2) | 5.20 |
| 2 | 5.71 | 3.39 | 2.32 | 9.49 | 12.56 | 22.05 | 5.35 | 1.02 | 2) | 6.57 |

- 1) Depending on the cable gland used: values up to ± 1.18 in
- 2) Dependent on the respective process connection

Flange connections

Fixed flange ASME B16.5

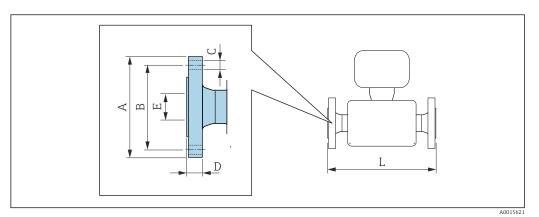

Length tolerance for dimension L in inch: +0.06 / -0.08

| Flange according to ASME B16.5: Cl 150 1.4404 (316/316L) Order code for "Process connection", option AAW | | | | | | |
|--|-----------|-----------|-----------|-----------|-----------|-----------|
| DN [in] | A [in] | B [in] | C [in] | D [in] | E [in] | L [in] |
| 3/8 1) | 3.54 | 2.37 | 4 × Ø0.62 | 0.50 | 0.62 | 13.23 |
| 1/2 | 3.54 | 2.37 | 4 × Ø0.62 | 0.50 | 0.62 | 17.32 |
| 1 | 4.33 | 3.13 | 4 × Ø0.62 | 0.59 | 1.05 | 22.83 |
| 11/2 | 4.92 | 3.87 | 4 × Ø0.62 | 0.69 | 1.61 | 31.26 |
| 2 5.91 4.75 4 × Ø0.75 0.93 2.07 42.17 | | | | | | |
| Surface roughness (flange): Ra 125 to 248 µin | | | | | | |


1) DN $\frac{3}{8}$ " with DN $\frac{1}{2}$ " flanges as standard

| Flange according to ASME B16.5: Cl 300 1.4404 (316/316L) Order code for "Process connection", option ABW | | | | | | |
|--|-----------|-----------|-----------|-----------|-----------|-----------|
| DN [in] | A [in] | B [in] | C [in] | D [in] | E [in] | L [in] |
| 3/8 1) | 3.74 | 2.63 | 4 × Ø0.62 | 0.56 | 0.62 | 13.23 |
| 1/2 | 3.74 | 2.63 | 4 × Ø0.62 | 0.56 | 0.62 | 17.32 |
| 1 | 4.92 | 3.50 | 4 × Ø0.75 | 0.69 | 1.05 | 22.83 |
| 1½ | 6.10 | 4.50 | 4 × Ø0.88 | 0.81 | 1.61 | 31.26 |
| 2 | 6.50 | 5.00 | 8 × Ø0.75 | 0.93 | 2.07 | 42.17 |
| Surface roughness (flange): Ra 125 to 248 µin | | | | | | |

1) DN $\frac{3}{8}$ " with DN $\frac{1}{2}$ " flanges as standard

Accessories


Rinse connections

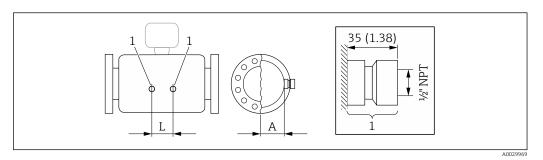


1 Connection nipple for purge connections: order code for "Sensor options", option CH "Purge connection"

| DN | A | L |
|------|------|-------|
| [in] | [in] | [in] |
| 3/8 | 1.85 | 4.33 |
| 1/2 | 1.85 | 8.03 |
| 1 | 1.85 | 13.7 |
| 1½ | 2.64 | 20.71 |
| 2 | 3.33 | 30.04 |

Protective cover

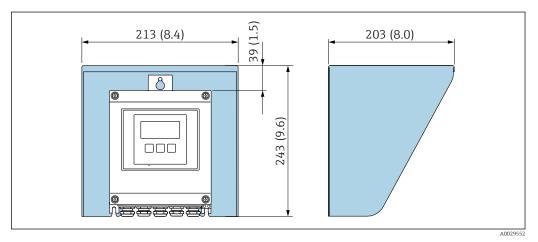

 \blacksquare 39 Weather protection cover for Proline 500 – digital

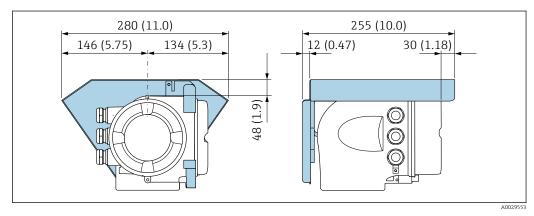


■ 40 Weather protection cover for Proline 500

External WLAN antenna

The external WLAN antenna is not suitable for use in hygienic applications.

Proline 500 – digital


External WLAN antenna mounted on device

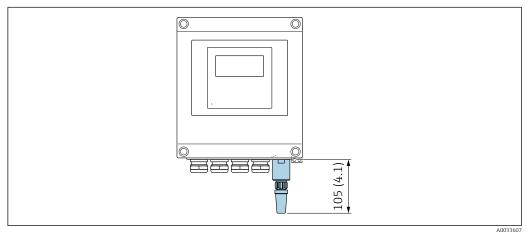

■ 41 Engineering unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

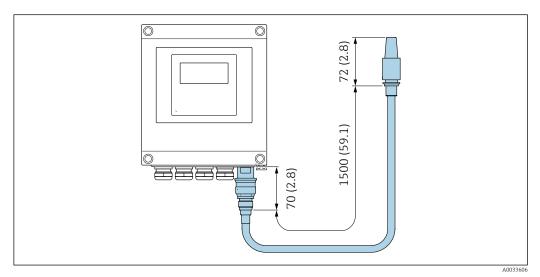


■ 42 Engineering unit mm (in)

Endress+Hauser 75

.....

Proline 500


External WLAN antenna mounted on device

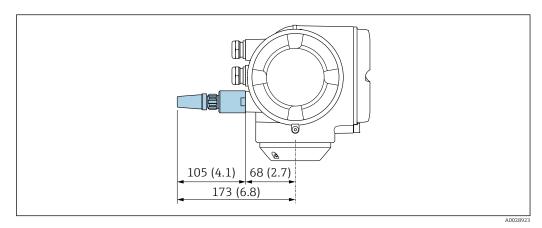

■ 43 Engineering unit mm (in)

External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.

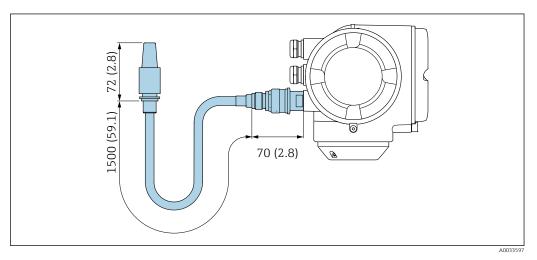

🛮 44 Engineering unit mm (in)

Weight

All values (weight exclusive of packaging material) refer to devices with EN/DIN PN 40 flanges.

Transmitter

- Proline 500 digital polycarbonate: 1.4 kg (3.1 lbs)
- Proline 500 digital aluminum: 2.4 kg (5.3 lbs)
- Proline 500 aluminum: 6.5 kg (14.3 lbs)
- Proline 500 cast, stainless: 15.6 kg (34.4 lbs)

Sensor

- Sensor with aluminum connection housing version: see the information in the following table
- Cast connection housing version, stainless: +3.7 kg (+8.2 lbs)

Weight in SI units

| DN [mm] | Weight [kg] |
|------------|-------------|
| 8 | 10 |
| 15 | 11 |
| 25 | 17 |

| DN [mm] | Weight [kg] | |
|------------|-------------|--|
| 40 | 34 | |
| 50 | 67 | |

Weight in US units

| DN [in] | Weight [lbs] |
|------------|--------------|
| 3/8 | 22 |
| 1/2 | 24 |
| 1 | 37 |
| 1½ | 75 |
| 2 | 148 |

Materials

Transmitter housing

Housing of Proline 500 – digital transmitter

Order code for "Transmitter housing":

- Option A "Aluminum coated": aluminum, AlSi10Mg, coated
- Option **D** "Polycarbonate": polycarbonate

Housing of Proline 500 transmitter

Order code for "Transmitter housing":

- Option **A** "Aluminum coated": aluminum, AlSi10Mg, coated
- \blacksquare Option L "Cast, stainless": cast, stainless steel, 1.4409 (CF3M) similar to 316L

Window material

Order code for "Transmitter housing":


- Option A "Aluminum, coated": glass
- Option **D** "Polycarbonate": plastic
- Option L "Cast, stainless": glass

Sensor connection housing

Order code for "Sensor connection housing":

- Option A "Aluminum coated": aluminum, AlSi10Mg, coated
- Option **B** "Stainless":
 - Stainless steel 1.4301 (304)
 - Optional: Order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel, 1.4404 (316L)
- Option **C** "Ultra-compact, stainless":
 - Stainless steel 1.4301 (304)
 - Optional: Order code for "Sensor feature", option CC "Hygienic version, for maximum corrosion resistance": stainless steel, 1.4404 (316L)
- Option L "Cast, stainless": 1.4409 (CF3M) similar to 316L

Cable entries/cable glands

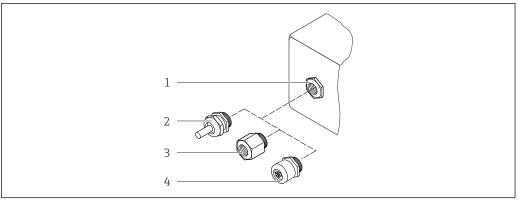

Possible cable entries/cable glands

- Female thread M20 \times 1.5
- Cable gland M20 \times 1.5 Adapter for cable entry with internal thread G $\frac{1}{2}$ " or NPT $\frac{1}{2}$ " 3
- Device plugs

| Cable entries and adapters | Material |
|---|--------------------------------|
| Cable gland M20 × 1.5 | Plastic |
| Adapter for cable entry with internal thread G ½" Adapter for cable entry with internal thread NPT ½" | Nickel-plated brass |
| Only available for certain device versions: Order code for "Transmitter housing": Option A "Aluminum, coated" Order code for "Sensor connection housing": Proline 500 – digital: Option A "Aluminum coated" Option B "Stainless" Option L "Cast, stainless" Option B "Stainless" Option B "Stainless" Option L "Cast, stainless" Option L "Cast, stainless" | |
| Adapter for cable entry with internal thread G ½" Adapter for cable entry with internal thread NPT ½" | Stainless steel, 1.4404 (316L) |
| Only available for certain device versions: Order code for "Transmitter housing": Option L "Cast, stainless" Order code for "Sensor connection housing": Option L "Cast, stainless" | |
| Adapter for device plug | Stainless steel, 1.4404 (316L) |
| Device plug for digital communication: Only available for certain device versions → ■ 29. | |

Device plug

| Electrical connection | Material | |
|-----------------------|---|--|
| Plug M12x1 | Socket: Stainless steel, 1.4404 (316L) Contact housing: Polyamide Contacts: Gold-plated brass | |


Connecting cable

Connecting cable for sensor - Proline 500 - digital transmitter

PVC cable with copper shield

Connecting cable for sensor - Proline 500 transmitter

- Standard cable: PVC cable with copper shield
- Reinforced cable: PVC cable with copper shield and additional steel wire braided jacket



Sensor housing


- Acid and alkali-resistant outer surface
- Stainless steel 1.4301 (304)

Measuring tubes

- Zirconium 702/R 60702
- Tantalum 2.5W

Process connections

- Stainless steel, 1.4301 (304); wetted parts: zirconium 702, tantalum
- Flanges according to EN 1092-1 (DIN 2501) / according to ASME B16.5 / according to JIS B2220



Seals

Welded process connections without internal seals

Accessories

Protective cover

Stainless steel, 1.4404 (316L)


External WLAN antenna

- Antenna: ASA plastic (acrylic ester-styrene-acrylonitrile) and nickel-plated brass
- Adapter: Stainless steel and nickel-plated brass
- Cable: Polyethylene
- Plug: Nickel-plated brass
- Angle bracket: Stainless steel

Process connections

Fixed flange connections:

- EN 1092-1 (DIN 2501) flange
- EN 1092-1 (DIN 2512N) flange
- ASME B16.5 flange
- JIS B2220 flange



Surface roughness

All data relate to parts in contact with fluid. The following surface roughness quality can be ordered. Not polished

Operability

Operating concept

Operator-oriented menu structure for user-specific tasks

- Commissioning
- Operation
- Diagnostics
- Expert level

Fast and safe commissioning

- Guided menus ("Make-it-run" wizards) for applications
- Menu guidance with brief descriptions of the individual parameter functions
- Device access via Web server or SmartBlue app \rightarrow 🖺 100
- WLAN access to the device via mobile handheld terminal, tablet or smart phone

Reliable operation

- Operation in local language → 🖺 80
- Uniform operating philosophy applied to device and operating tools
- If replacing electronic modules, transfer the device configuration via the integrated memory (HistoROM backup) which contains the process and measuring device data and the event logbook. No need to reconfigure.

Efficient diagnostics increase measurement availability

- Troubleshooting measures can be called up via the device and in the operating tools
- Diverse simulation options, logbook for events that occur and optional line recorder functions

Languages

Can be operated in the following languages:

- Via local operation
 English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese,
 Japanese, Korean, Bahasa (Indonesian), Vietnamese, Czech, Swedish
- Via Web browser
 English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Korean, Bahasa (Indonesian), Vietnamese, Czech, Swedish
- Via "FieldCare", "DeviceCare" operating tool: English, German, French, Spanish, Italian, Chinese, Japanese

Local operation


Via display module

Two display modules are available:

- Order code for "Display; operation", option F "4-line, illuminated, graphic display; touch control"
- Order code for "Display; operation", option G "4-line, illuminated, graphic display; touch control + WLAN"



Information about WLAN interface → 🖺 87

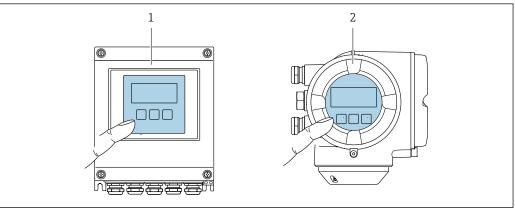

A002823

■ 46 Operation with touch control

- 1 Proline 500 digital
- 2 Proline 500

80

Display elements

- 4-line, illuminated, graphic display
- White background lighting; switches to red in event of device errors
- Format for displaying measured variables and status variables can be individually configured
- Permitted ambient temperature for the display: -20 to +60 °C (-4 to +140 °F)
 The readability of the display may be impaired at temperatures outside the temperature range.


Operating elements

- External operation via touch control (3 optical keys) without opening the housing: \boxdot , \boxdot , \boxdot
- Operating elements also accessible in the various zones of the hazardous area

Remote operation

Via HART protocol

This communication interface is available in device versions with a HART output.

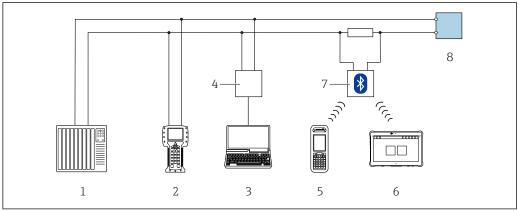


■ 47 Options for remote operation via HART protocol (active)

- 1 Control system (e.g. PLC)
- 2 Field Communicator 475
- 3 Computer with Web browser (e.g. Internet Explorer) for access to the integrated device Web server or computer with an operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 4 Commubox FXA195 (USB)
- 5 Field Xpert SFX350 or SFX370
- 6 Field Xpert SMT70
- 7 VIATOR Bluetooth modem with connecting cable
- 3 Transmitter

Endress+Hauser 81

A0028747

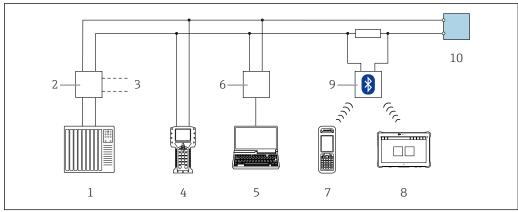


A002874

■ 48 Options for remote operation via HART protocol (passive)

- 1 Control system (e.g. PLC)
- 2 Transmitter power supply unit, e.g. RN221N (with communication resistor)
- 3 Connection for Commubox FXA195 and Field Communicator 475
- 4 Field Communicator 475
- 5 Computer with Web browser (e.g. Internet Explorer) for access to the integrated device Web server or computer with an operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 6 Commubox FXA195 (USB)
- 7 Field Xpert SFX350 or SFX370
- 8 Field Xpert SMT70
- 9 VIATOR Bluetooth modem with connecting cable
- 10 Transmitter

Via FOUNDATION Fieldbus network

This communication interface is available in device versions with FOUNDATION Fieldbus.

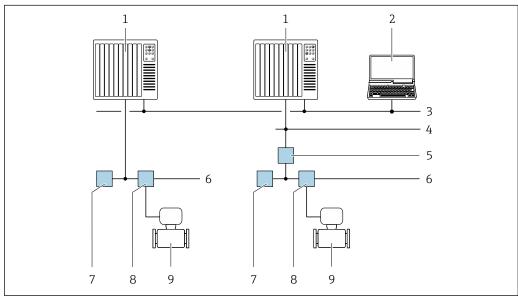


A002883

■ 49 Options for remote operation via FOUNDATION Fieldbus network

- 1 Automation system
- 2 Computer with FOUNDATION Fieldbus network card
- 3 Industry network
- 4 High Speed Ethernet FF-HSE network
- 5 Segment coupler FF-HSE/FF-H1
- 6 FOUNDATION Fieldbus FF-H1 network
- 7 Power supply FF-H1 network
- 8 T-box
- 9 Measuring device

Via PROFIBUS DP network

This communication interface is available in device versions with PROFIBUS DP.

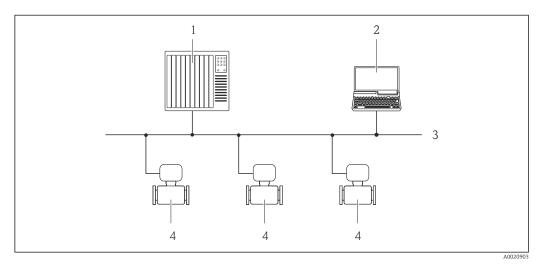


 \blacksquare 50 Options for remote operation via PROFIBUS DP network

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Measuring device

Via PROFIBUS PA network

This communication interface is available in device versions with PROFIBUS PA.

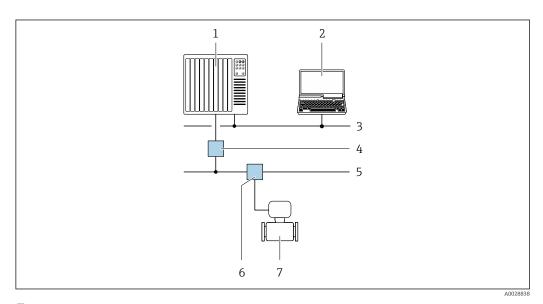


■ 51 Options for remote operation via PROFIBUS PA network

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Segment coupler PROFIBUS DP/PA
- 5 PROFIBUS PA network
- 6 T-box
- 7 Measuring device

Via Modbus RS485 protocol

This communication interface is available in device versions with a Modbus-RS485 output.

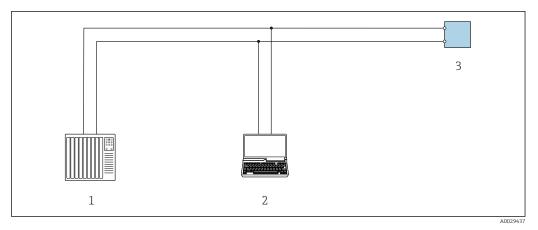


 \blacksquare 52 Options for remote operation via Modbus-RS485 protocol (active)

- 1 Control system (e.g. PLC)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 3 Transmitter

Via EtherNet/IP network

This communication interface is available in device versions with EtherNet/IP.

Star topology

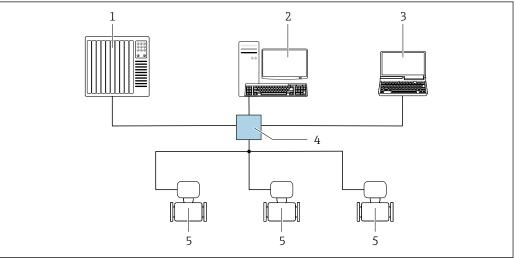


A0032078

■ 53 Options for remote operation via EtherNet/IP network: star topology

- 1 Automation system, e.g. "RSLogix" (Rockwell Automation)
- 2 Workstation for measuring device operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Ethernet switch
- 5 Measuring device

Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).

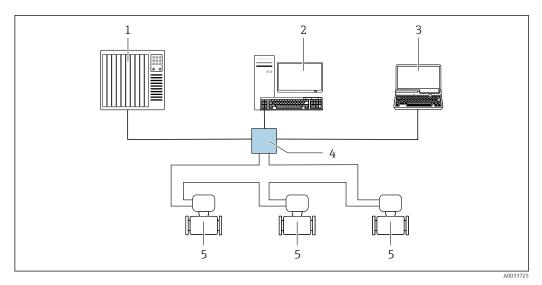


■ 54 Options for remote operation via EtherNet/IP network: ring topology

- 1 Automation system, e.g. "RSLogix" (Rockwell Automation)
- 2 Workstation for measuring device operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Ethernet switch
- 5 Measuring device

Via PROFINET network

This communication interface is available in device versions with PROFINET.

Star topology

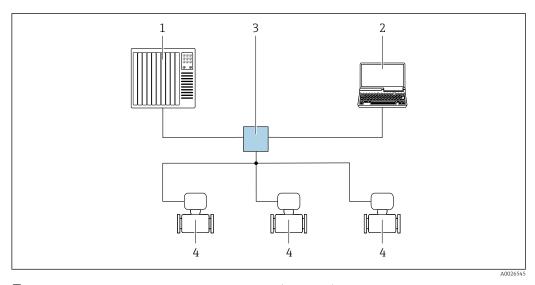


■ 55 Options for remote operation via PROFINET network: star topology

- Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Switch, e.g. Scalance X204 (Siemens)
- 4 Measuring device

Ring topology

This communication interface is available in device versions with PROFINET.

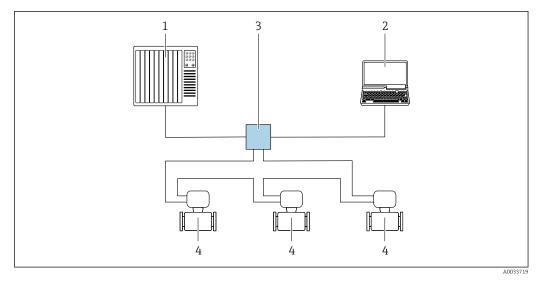


■ 56 Options for remote operation via PROFINET network: ring topology

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Switch, e.g. Scalance X204 (Siemens)
- 4 Measuring device

Service interface


Via service interface (CDI-RJ45)

A point-to-point connection can be established to configure the device onsite. With the housing open, the connection is established directly via the service interface (CDI-RJ45) of the device.



The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. Therefore the connection to the service interface can be established via an M12 connector without opening the device.


Proline 500 – digital transmitter

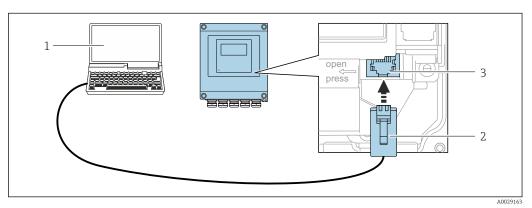

■ 57 Connection via service interface (CDI-RJ45)

- 1 Computer with Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or with "FieldCare", "DeviceCare" operating tool with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 2 Standard Ethernet connecting cable with RJ45 connector
- Service interface (CDI-RJ45) of the measuring device with access to the integrated Web server

Proline 500 transmitter

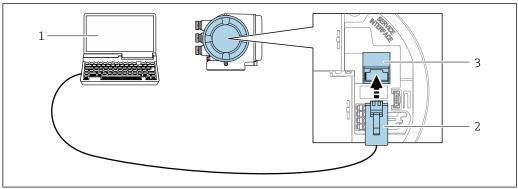


Connection via service interface (CDI-RJ45)

- Computer with Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or with "FieldCare", "DeviceCare" operating tool with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- Standard Ethernet connecting cable with RJ45 connector
- Service interface (CDI-RJ45) of the measuring device with access to the integrated Web server

Via WLAN interface

The optional WLAN interface is available on the following device version: Order code for "Display; operation", option G "4-line, illuminated, graphic display; touch control +

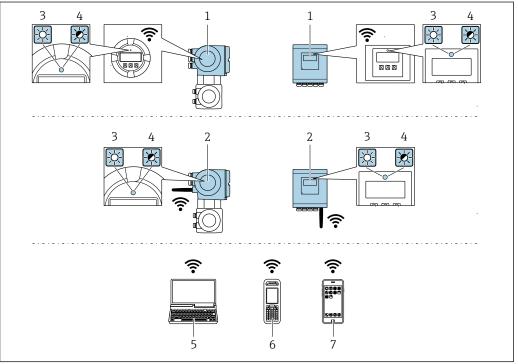

A0034569

- Transmitter with integrated WLAN antenna
- 2 Transmitter with external WLAN antenna
- 3 LED lit constantly: WLAN reception is enabled on measuring device
- LED flashing: WLAN connection established between operating unit and measuring device
- Computer with WLAN interface and Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or with operating tool (e.g. FieldCare, DeviceCare)
- Mobile handheld terminal with WLAN interface and Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or operating tool (e.g. FieldCare, DeviceCare)


Smart phone or tablet (e.g. Field Xpert SMT70)

| Function | WLAN: IEEE 802.11 b/g (2.4 GHz) • Access point with DHCP server (default setting) • Network |
|-------------------------------------|---|
| Encryption | WPA2-PSK AES-128 (in accordance with IEEE 802.11i) |
| Configurable WLAN channels | 1 to 11 |
| Degree of protection | IP67 |
| Available antennas | Internal antenna External antenna (optional) In the event of poor transmission/reception conditions at the place of installation. Available as an accessory → □ 98. Only one antenna active in each case! |
| Max. range | 50 m (164 ft) |
| Materials: External WLAN antenna | Antenna: ASA plastic (acrylic ester-styrene-acrylonitrile) and nickel-plated brass Adapter: Stainless steel and nickel-plated brass Cable: Polyethylene Connector: Nickel-plated brass Angle bracket: Stainless steel |

Network integration

With the optional OPC-UA-Server application package, the device can be integrated into an Ethernet network via the service interface (CDI-RJ45 and WLAN) and communicate with OPC-UA clients. If the device is used in this way, IT security must be considered.

For permanent access to device data and for device configuration via the Web server, the device is incorporated directly in a network via the service interface (CDI-RJ45). In this way, the device can be accessed any time from the control station. The measured values are processed separately via the inputs and outputs through the automation system.

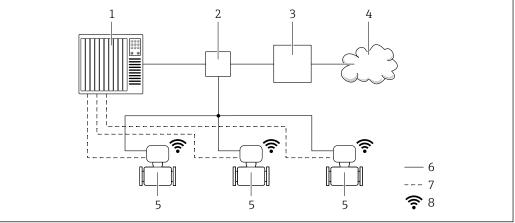

A003361

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch
- 3 Edge Gateway
- 4 Cloud
- 5 Measuring device
- 6 Ethernet network
- 7 Measured values via inputs and outputs
- 8 Optional WLAN interface
- The optional WLAN interface is available on the following device version:

 Order code for "Display; operation", option **G** "4-line, illuminated, graphic display; touch control +

Supported operating tools

Different operating tools can be used for local or remote access to the measuring device. Depending on the operating tool used, access is possible with different operating units and via a variety of interfaces.

| Supported operating tools | Operating unit | Interface | Additional information |
|---------------------------|--|---|--|
| Web browser | Notebook, PC or tablet with Web browser | CDI-RJ45 service interface WLAN interface Ethernet-based fieldbus (EtherNet/IP, PROFINET) | Special Documentation for device → 🖺 102 |
| DeviceCare SFE100 | Notebook, PC or tablet with Microsoft Windows system | CDI-RJ45 service interfaceWLAN interfaceFieldbus protocol | → 🖺 100 |
| FieldCare SFE500 | Notebook, PC or tablet with Microsoft Windows system | CDI-RJ45 service interfaceWLAN interfaceFieldbus protocol | → 🖺 100 |
| Device Xpert | Field Xpert SFX 100/350/370 | HART and FOUNDATION Fieldbus fieldbus protocol | Operating Instructions BA01202S Device description files: Use update function of handheld terminal |

- i
- Other operating tools based on FDT technology with a device driver such as DTM/iDTM or DD/EDD can be used for device operation. These operating tools are available from the individual manufacturers. Integration into the following operating tools, among others, is supported:
- FactoryTalk AssetCentre (FTAC) by Rockwell Automation → www.rockwellautomation.com
- Process Device Manager (PDM) by Siemens → www.siemens.com
- Asset Management Solutions (AMS) by Emerson → www.emersonprocess.com
- FieldCommunicator 375/475 by Emerson → www.emersonprocess.com
- Field Device Manager (FDM) by Honeywell → www.honeywellprocess.com
- FieldMate by Yokogawa → www.yokogawa.com
- PACTWare → www.pactware.com

The associated device description files are available at: www.endress.com → Downloads

Web server

Thanks to the integrated Web server, the device can be operated and configured via a Web browser and via a service interface (CDI-RJ45) or via a WLAN interface. The structure of the operating menu is the same as for the local display. In addition to the measured values, status information on the device is also displayed and allows the user to monitor the status of the device. Furthermore the device data can be managed and the network parameters can be configured.

A device that has a WLAN interface (can be ordered as an option) is required for the WLAN connection: order code for "Display; operation", option $\bf G$ "4-line, illuminated; touch control + WLAN". The device acts as an Access Point and enables communication by computer or a mobile handheld terminal.

Supported functions

Data exchange between the operating unit (such as a notebook for example) and the measuring device:

- Upload the configuration from the measuring device (XML format, configuration backup)
- Save the configuration to the measuring device (XML format, restore configuration)
- Export event list (.csv file)
- Export parameter settings (.csv file or PDF file, document the measuring point configuration)
- Export the Heartbeat verification log (PDF file, only available with the "Heartbeat Verification" application package)

- Flash firmware version for device firmware upgrade, for instance
- Download driver for system integration



Web server special documentation \rightarrow $\stackrel{\triangle}{=}$ 102

HistoROM data management

The measuring device features HistoROM data management. HistoROM data management comprises both the storage and import/export of key device and process data, making operation and servicing far more reliable, secure and efficient.



When the device is delivered, the factory settings of the configuration data are stored as a backup in the device memory. This memory can be overwritten with an updated data record, for example after commissioning.

Additional information on the data storage concept

There are different types of data storage units in which device data are stored and used by the device:

| | Device memory | T-DAT | S-DAT |
|------------------|---|--|---|
| Available data | Event logbook such as diagnostic events for example Parameter data record backup Device firmware package Driver for system integration for exporting via Web server, e.g: GSD for PROFIBUS DP GSD for PROFIBUS PA GSDML for PROFINET EDS for EtherNet/IP DD for FOUNDATION Fieldbus | Measured value logging ("Extended HistoROM" order option) Current parameter data record (used by firmware at run time) Peakhold indicator (min/max values) Totalizer values | Sensor data: nominal diameter etc. Serial number Calibration data Device configuration (e.g. SW options, fixed I/O or multi I/O) |
| Storage location | Fixed on the user interface board in the connection compartment | Attachable to the user interface board in the connection compartment | In the sensor plug in the transmitter neck part |

Data backup

Automatic

- The most important device data (sensor and transmitter) are automatically saved in the DAT modules
- If the transmitter or measuring device is replaced: once the T-DAT containing the previous device data has been exchanged, the new measuring device is ready for operation again immediately without any errors
- If the sensor is replaced: once the sensor has been replaced, new sensor data are transferred from the S-DAT in the measuring device and the measuring device is ready for operation again immediately without any errors
- If exchanging the electronics module (e.g. I/O electronics module): Once the electronics module has been replaced, the software of the module is compared against the current device firmware. The module software is upgraded or downgraded where necessary. The electronics module is available for use immediately afterwards and no compatibility problems occur.

Manual

Additional parameter data record (complete parameter settings) in the integrated device memory HistoROM backup for:

- Data backup function
 Backup and subsequent restoration of a device configuration in the device memory HistoROM backup
- Data comparison function
 Comparison of the current device configuration with the device configuration saved in the device memory HistoROM backup

Data transfer

Manual

- Transfer of a device configuration to another device using the export function of the specific operating tool, e.g. with FieldCare, DeviceCare or Web server: to duplicate the configuration or to store in an archive (e.g. for backup purposes)
- Transmission of the drivers for system integration via Web server, e.g.:
 - GSD for PROFIBUS DP
 - GSD for PROFIBUS PA
 - GSDML for PROFINET
 - EDS for EtherNet/IP
 - DD for FOUNDATION Fieldbus

Event list

Automatic

- Chronological display of up to 20 event messages in the events list
- If the Extended HistoROM application package (order option) is enabled: up to 100 event messages are displayed in the events list along with a time stamp, plain text description and remedial measures
- The events list can be exported and displayed via a variety of interfaces and operating tools e.g. DeviceCare, FieldCare or Web server

Data logging

Manual

If the **Extended HistoROM** application package (order option) is enabled:

- Record up to 1000 measured values via 1 to 4 channels
- User configurable recording interval
- Record up to 250 measured values via each of the 4 memory channels
- Export the measured value log via a variety of interfaces and operating tools e.g. FieldCare, DeviceCare or web server

Certificates and approvals



Currently available certificates and approvals can be called up via the product configurator.

CE mark

The device meets the legal requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied.

Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.

C-Tick symbol


The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".

Ex approval

The measuring device is certified for use in hazardous areas and the relevant safety instructions are provided in the separate "Safety Instructions" (XA) document. Reference is made to this document on the nameplate.

The following devices have equipment protection level (EPL) Gb (Zone 1 in the measuring tube):

- Device versions with the order code for "Integrated ISEM electronics", option A and the order code for "Approval; transmitter; sensor", option BI, BJ, BM or BN.
- Device versions with the order code for "Integrated ISEM electronics", option B and the order code for "Approval; transmitter; sensor", option BA, BB, BC or BD.



Proline 500 - digital

ATEX/IECEx

Currently, the following versions for use in hazardous areas are available:

Ex ia

| | Transmitter | Sensor | | |
|----------|---------------------------|----------|--|--|
| Category | Type of protection | Category | Type of protection | |
| II(1)G | [Ex ia] IIC | II1/2G | Ex ia IIC T6T1 Gb Ex ia IIB T6T1 Gb | |
| II(1)G | [Ex ia] IIC | II2G | Ex ia IIC T6T1 Gb Ex ia IIB T6T1 Gb | |
| II3(1)G | Ex ec [ia Ga] IIC T5T4 Gc | II1/2G | Ex ia IIC T6T1 Gb Ex ia IIB T6T1 Gb | |
| II3(1)G | Ex ec [ia Ga] IIC T5T4 Gc | II2G | Ex ia IIC T6T1 Gb Ex ia IIB T6T1 Gb | |

Ex tb

| Transmitter | | Sensor | |
|-------------|--------------------|----------|-------------------------|
| Category | Type of protection | Category | Type of protection |
| II(1)D | [Ex ia] IIIC | II2D | Ex ia tb IIIC T** °C Db |

Non-Ex / Ex ec

| Transmitter | | Sensor | |
|-------------|--------------------|----------|--------------------|
| Category | Type of protection | Category | Type of protection |
| Non - Ex | Non-Ex | II3G | Ex ec IIC T5T1 Gc |
| II3G | Ex ec IIC T5T4 Gc | II3G | Ex ec IIC T5T1 Gc |

$_{C}CSA_{US}$

Currently, the following versions for use in hazardous areas are available:

IS (Ex nA, Ex i)

| Transmitter | Sensor |
|---------------------------------|--|
| Class I Division 2 Groups A - D | Class I, II, III Division 1 Groups A-G |
| Class I Division 2 Groups A - D | Class I, II, III Division 1 Groups C-G |

NI (Ex nA)

| Transmitter | Sensor |
|---------------------------|--------|
| Class I Division 2 Groups | A - D |

Ex nA / Ex i

| Transmitter | Sensor |
|--|--|
| Class I, Zone 2 AEx/ Ex nA [ia Ga] IIC T5T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |
| Class I, Zone 2 AEx/ Ex nA [ia Ga] IIC T5T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |

Ex nA

| Transmitter | Sensor |
|--|--|
| Class I, Zone 2 AEx/ Ex nA IIC T5T4 Gc | Class I, Zone 2 AEx/ Ex nA IIC T5T1 Gc |

Ex tb

| Transmitter | Sensor |
|---------------------|--------------------------------------|
| [AEx / Ex ia] IIIC | Zone 21 AEx/ Ex ia tb IIIC T** °C Db |

Proline 500

ATEX/IECEx

Currently, the following versions for use in hazardous areas are available:

Ex db eb

| Transmitter | | Sensor | |
|-------------|-------------------------|----------|--------------------|
| Category | Type of protection | Category | Type of protection |
| II2G | Ex db eb ia IIC T6T4 Gb | II2G | Ex ia IIC T6T1 Gb |
| II2G | Ex db eb ia IIB T6T4 Gb | II2G | Ex ia IIB T6T1 Gb |
| II2G | Ex db eb ia IIC T6T4 Gb | II2G | Ex ia IIC T6T1 Gb |
| II2G | Ex db eb ia IIB T6T4 Gb | II2G | Ex ia IIB T6T1 Gb |

Ex db

| Transmitter | | Sensor | |
|-------------|----------------------|----------|--------------------|
| Category | Type of protection | Category | Type of protection |
| II2G | Ex db ia IIC T6T4 Gb | II2G | Ex ia IIC T6T1 Gb |
| II2G | Ex db ia IIB T6T4 Gb | II2G | Ex ia IIB T6T1 Gb |
| II2G | Ex db ia IIC T6T4 Gb | II2G | Ex ia IIC T6T1 Gb |
| II2G | Ex db ia IIB T6T4 Gb | II2G | Ex ia IIB T6T1 Gb |

Ex tb

| Category | Type of protection | |
|----------|---------------------|-------------------------|
| | Transmitter Sensor | |
| II2D | Ex tb IIIC T85°C Db | Ex ia tb IIIC T** °C Db |

Ех ес

| Category | Type of protection | |
|----------|--------------------|-------------------|
| | Transmitter | Sensor |
| II3G | Ex ec IIC T5T4 Gc | Ex ec IIC T5T1 Gc |

$_{C}CSA_{US}$

Currently, the following versions for use in hazardous areas are available:

IS (Ex i) and XP (Ex d)

| Transmitter | Sensor | |
|---|--------|--|
| Class I, III, III Division 1 Groups A-G | | |
| Class I, III, III Division 1 Groups C-G | | |

NI (Ex nA)

| Transmitter | Sensor |
|---------------------------|--------|
| Class I Division 2 Groups | ABCD |

Ex de

| Transmitter | Sensor |
|---|--|
| Class I, Zone 1 AEx/ Ex de ia IIC T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb |
| Class I, Zone 1 AEx/ Ex de ia IIB T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |
| Class I, Zone 1 AEx/ Ex de ia IIC T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb |
| Class I, Zone 1 AEx/ Ex de ia IIB T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |

Ex d

| Transmitter | Sensor |
|--|--|
| Class I, Zone 1 AEx/ Ex d ia IIC T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb |
| Class I, Zone 1 AEx/ Ex d ia IIB T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |
| Class I, Zone 1 AEx/ Ex d ia IIC T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIC T6T1 Gb |
| Class I, Zone 1 AEx/ Ex d ia IIB T6T4 Gb | Class I, Zone 1 AEx/ Ex ia IIB T6T1 Gb |

Ex nA

| Transmitter | Sensor |
|--|--|
| Class I, Zone 2 AEx/ Ex nA IIC T5T4 Gc | Class I, Zone 2 AEx/ Ex nA IIC T5T1 Gc |

Ex tb

| Transmitter | Sensor |
|----------------------------------|--------------------------------------|
| Zone 21 AEx/ Ex tb IIIC T85°C Db | Zone 21 AEx/ Ex ia tb IIIC T** °C Db |

Pharmaceutical compatibility


- FDA
- USP Class VI
- TSE/BSE Certificate of Suitability

Functional safety

The measuring device can be used for flow monitoring systems (min., max., range) up to SIL 2 (single-channel architecture; order code for "Additional approval", option LA) and SIL 3 (multichannel architecture with homogeneous redundancy) and is independently evaluated and certified by the $T\ddot{U}V$ in accordance with IEC 61508.

The following types of monitoring in safety equipment are possible:

- Mass flow
- Volume flow
- Density



HART certification

HART interface

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified according to HART 7
- The device can also be operated with certified devices of other manufacturers (interoperability)

FOUNDATION Fieldbus certification

FOUNDATION Fieldbus interface

The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified in accordance with FOUNDATION Fieldbus H1
- Interoperability Test Kit (ITK), revision version 6.2.0 (certificate available on request)
- Physical Layer Conformance Test
- The device can also be operated with certified devices of other manufacturers (interoperability)

Certification PROFIBUS

PROFIBUS interface

The measuring device is certified and registered by the PNO (PROFIBUS User Organization Organization). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with PROFIBUS PA Profile 3.02
- The device can also be operated with certified devices of other manufacturers (interoperability)

EtherNet/IP certification

The measuring device is certified and registered by the ODVA (Open Device Vendor Association). The measuring system meets all the requirements of the following specifications:

- Certified in accordance with the ODVA Conformance Test
- EtherNet/IP Performance Test
- EtherNet/IP PlugFest compliance
- The device can also be operated with certified devices of other manufacturers (interoperability)

Certification PROFINET

PROFINET interface

The measuring device is certified and registered by the PNO (PROFIBUS User Organization Organization). The measuring system meets all the requirements of the following specifications:

- Certified according to:
 - Test specification for PROFINET devices
 - PROFINET Security Level 2 Netload Class
- The device can also be operated with certified devices of other manufacturers (interoperability)

Pressure Equipment Directive

The devices can be ordered with or without a PED approval. If a device with a PED approval is required, this must be explicitly stated in the order. For devices with nominal diameters less than or equal to DN 25 (1"), this is neither possible nor necessary.

- With the identification PED/G1/x (x = category) on the sensor nameplate, Endress+Hauser confirms conformity with the "Essential Safety Requirements" specified in Appendix I of the Pressure Equipment Directive 2014/68/EU.
- Devices bearing this marking (PED) are suitable for the following types of medium:
 - Media in Group 1 and 2 with a vapor pressure greater than, or smaller and equal to 0.5 bar (7.3 psi)
 - Unstable gases
- Devices not bearing this marking (PED) are designed and manufactured according to good engineering practice. They meet the requirements of Article 4 paragraph 3 of the Pressure Equipment Directive 2014/68/EU. The range of application is indicated in tables 6 to 9 in Annex II of the Pressure Equipment Directive 2014/68/EU.

Radio approval

The measuring device has radio approval.



For detailed information on the radio approval, see the Special Documentation $\rightarrow \implies 102$

Additional certification

CRN approval

Some device versions have CRN approval. A CRN-approved process connection with a CSA approval must be ordered for a CRN-approved device.

Tests and certificates

- Pressure test, internal procedure, inspection certificate
- EN10204-3.1 material certificate, wetted parts and sensor housing
- PMI test (XRF), internal procedure, wetted parts, test report
- EN10204-2.1 confirmation of compliance with the order and EN10204-2.2 test report

Other standards and quidelines

■ EN 60529

Degrees of protection provided by enclosures (IP code)

■ IEC/EN 60068-2-6

Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal).

■ IEC/EN 60068-2-31

Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.

■ EN 61010-1

Safety requirements for electrical equipment for measurement, control and laboratory use general requirements

■ IEC/EN 61326

Emission in accordance with Class A requirements. Electromagnetic compatibility (EMC requirements).

■ NAMUR NE 21

Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment

NAMUR NE 32

Data retention in the event of a power failure in field and control instruments with microprocessors

■ NAMUR NE 43

Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.

■ NAMUR NE 53

Software of field devices and signal-processing devices with digital electronics

■ NAMUR NE 80

The application of the pressure equipment directive to process control devices

■ NAMUR NE 105

Specifications for integrating fieldbus devices in engineering tools for field devices

■ NAMUR NE 107

Self-monitoring and diagnosis of field devices

■ NAMUR NE 131

Requirements for field devices for standard applications

■ NAMUR NE 132

Coriolis mass meter

Ordering information

Detailed ordering information is available from the following sources:

- In the Product Configurator on the Endress+Hauser website: www.endress.com -> Click "Corporate" -> Select your country -> Click "Products" -> Select the product using the filters and search field -> Open product page -> The "Configure" button to the right of the product image opens the Product Configurator.
- From your Endress+Hauser Sales Center: www.addresses.endress.com

Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.



Detailed information on the application packages: Special Documentation for the device $\rightarrow \triangleq 102$

| Diagnostics functions | Package | Description |
|-----------------------|---------------------------------------|---|
| | Extended HistoROM | Comprises extended functions concerning the event log and the activation of the measured value memory. |
| | | Event log: Memory volume is extended from 20 message entries (standard version) to up to 100 entries. |
| | | Data logging (line recorder): Memory capacity for up to 1000 measured values is activated. 250 measured values can be output via each of the 4 memory channels. The recording interval can be defined and configured by the user. Measured value logs can be accessed via the local display or operating tool e.g. FieldCare, DeviceCare or Web server. |
| Heartbeat Technology | Package | Description |
| | - | - |
| | Heartbeat Verification +Monitoring | Heartbeat Verification Meets the requirement for traceable verification to DIN ISO 9001:2008 Chapter 7.6 a) "Control of monitoring and measuring equipment". Functional testing in the installed state without interrupting the process. Traceable verification results on request, including a report. Simple testing process via local operation or other operating interfaces. Clear measuring point assessment (pass/fail) with high test coverage within the framework of manufacturer specifications. Extension of calibration intervals according to operator's risk assessment. |
| | | Heartbeat Monitoring Continuously supplies data, which are characteristic of the measuring principle, to an external condition monitoring system for the purpose of preventive maintenance or process analysis. These data enable the operator to: Draw conclusions - using these data and other information - about the impact process influences (such as corrosion, abrasion, buildup etc.) have on the measuring performance over time. Schedule servicing in time. Monitor the process or product quality, e.g. gas pockets. |
| | | |
| Concentration | Package | Description |
| | Concentration | Calculation and outputting of fluid concentrations |
| | | The measured density is converted to the concentration of a substance of a binary mixture using the "Concentration" application package: Choice of predefined fluids (e.g. various sugar solutions, acids, alkalis, salts, ethanol etc.) Common or user-defined units ("Brix, "Plato, % mass, % volume, mol/l etc.) for |
| | | standard applications.Concentration calculation from user-defined tables. |
| | | |
| Special density | Package | Description |
| | Special density | Many applications use density as a key measured value for monitoring quality or controlling processes. The device measures the density of the fluid as standard and makes this value available to the control system. The "Special Density" application package offers high-precision density measurement over a wide density and temperature range particularly for applications subject to varying process conditions. |
| OPC-UA server | | - |
| UPC-UA server | Package | Description |
| | OPC-UA-Server | The application package provides the user with an integrated OPC-UA server for comprehensive instrument services for IoT and SCADA applications. |
| | | |

Endress+Hauser 97

Accessories

Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: www.endress.com.

Device-specific accessories

For the transmitter

| Accessories | Description |
|--|---|
| Transmitter Proline 500 – digital Proline 500 | Transmitter for replacement or storage. Use the order code to define the following specifications: Approvals Output Input Display/operation Housing Software Proline 500 – digital transmitter: Order code: 8X5BXX-XXXXXXXXXX Proline 500 transmitter: Order code: 8X5BXX-XXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXXX |
| | Proline 500 transmitter for replacement: It is essential to specify the serial number of the current transmitter when ordering. Based on the serial number, the device-specific data (e.g., calibration factors) of the replacement device can be used for the new transmitter. Proline 500 – digital transmitter: Installation Instructions EA01151 Proline 500 transmitter: Installation Instructions EA01152 |
| External WLAN antenna | External WLAN antenna with 1.5 m (59.1 in) connecting cable and two angle brackets. Order code for "Enclosed accessories", option P8 "Wireless antenna wide area". ■ The external WLAN antenna is not suitable for use in hygienic applications. ■ Further information on the WLAN interface → ■ 87. ■ Order number: 71351317 ■ Installation Instructions EA01238D |
| Pipe mounting set | Pipe mounting set for transmitter. Proline 500 – digital transmitter Order number: 71346427 Proline 500 transmitter Order number: 71346428 |
| Protective cover Transmitter Proline 500 – digital Proline 500 | Is used to protect the measuring device from the effects of the weather: e.g. rainwater, excess heating from direct sunlight. Proline 500 – digital transmitter Order number: 71343504 Proline 500 transmitter Order number: 71343505 Installation Instructions EA01160 |
| Display guard Proline 500 – digital | Is used to protect the measuring device from the effects of the weather: e.g. rainwater, excess heating from direct sunlight. Order number: 71228792 For details, see Installation Instructions EA01093 |

| Connecting cable Proline 500 – digital Sensor – Transmitter | The connecting cable can be ordered directly with the measuring device (order code for "Cable, sensor connection) or as an accessory (order number DK8012). The following cable lengths are available: order code for "Cable, sensor connection" Option B: 20 m (65 ft) Option E: User configurable up to max. 50 m Option F: User configurable up to max. 165 ft |
|--|---|
| | Maximum possible cable length for a Proline 500 – digital connecting cable: 300 m (1000 ft) |
| Connecting cable Proline 500 Sensor – Transmitter | The connecting cable can be ordered directly with the measuring device (order code for "Cable, sensor connection) or as an accessory (order number DK8012). The following cable lengths are available: order code for "Cable, sensor connection" Option 1: 5 m (16 ft) |
| | Option 2: 10 m (32 ft) Option 3: 20 m (65 ft) |
| | Possible cable length for a Proline 500 connecting cable: max. 20 m (65 ft) |

For the sensor

| Accessories | Description |
|----------------|---|
| Heating jacket | Is used to stabilize the temperature of the fluids in the sensor. Water, water vapor and other non-corrosive liquids are permitted for use as fluids. |
| | If using oil as a heating medium, please consult with Endress+Hauser. |
| | Special Documentation SD02157D |

Communication-specific accessories

| Accessories | Description |
|------------------------------|--|
| Commubox FXA195 HART | For intrinsically safe HART communication with FieldCare via the USB interface. Technical Information TI00404F |
| HART Loop Converter HMX50 | Is used to evaluate and convert dynamic HART process variables to analog current signals or limit values. • Technical Information TI00429F • Operating Instructions BA00371F |
| Fieldgate FXA320 | Gateway for the remote monitoring of connected 4-20 mA measuring devices via a Web browser. Technical Information TI00025S Operating Instructions BA00053S |
| Fieldgate FXA520 | Gateway for the remote diagnostics and remote configuration of connected HART measuring devices via a Web browser. Technical Information TI00025S Operating Instructions BA00051S |
| Field Xpert SFX350 | Field Xpert SFX350 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices and can be used in non-hazardous areas. Operating Instructions BA01202S |

| Field Xpert SFX370 | Field Xpert SFX370 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices and can be used in the non-hazardous area and in the hazardous area. Operating Instructions BA01202S |
|--------------------|---|
| Field Xpert SMT70 | The Field Xpert SMT70 tablet PC for device configuration enables mobile plant asset management in hazardous and non-hazardous areas. It is suitable for commissioning and maintenance staff to manage field instruments with a digital communication interface and to record progress. This tablet PC is designed as an all-in-one solution with a preinstalled driver library and is an easy-to-use, touch-sensitive tool which can be used to manage field instruments throughout their entire life cycle. |
| | Technical Information TI01342S Operating Instructions BA01709S Product page: www.endress.com/smt70 |

Service-specific accessories

| Accessories | Description |
|-------------|---|
| Applicator | Software for selecting and sizing Endress+Hauser measuring devices: Choice of measuring devices for industrial requirements Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, flow velocity and accuracy. Graphic illustration of the calculation results Determination of the partial order code, administration, documentation and access to all project-related data and parameters over the entire life cycle of a project. |
| | Applicator is available: Via the Internet: https://portal.endress.com/webapp/applicator As a downloadable DVD for local PC installation. |
| W@M | W@M Life Cycle Management Improved productivity with information at your fingertips. Data relevant to a plant and its components is generated from the first stages of planning and during the asset's complete life cycle. W@M Life Cycle Management is an open and flexible information platform with online and on-site tools. Instant access for your staff to current, in-depth data shortens your plant's engineering time, speeds up procurement processes and increases plant uptime. Combined with the right services, W@M Life Cycle Management boosts productivity in every phase. For more information, visit www.endress.com/lifecyclemanagement |
| FieldCare | FDT-based plant asset management tool from Endress+Hauser. It can configure all smart field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition. Operating Instructions BA00027S and BA00059S |
| DeviceCare | Tool to connect and configure Endress+Hauser field devices. Innovation brochure IN01047S |

System components

| Accessories | Description |
|----------------------------------|---|
| Memograph M graphic data manager | The Memograph M graphic data manager provides information on all the relevant measured variables. Measured values are recorded correctly, limit values are monitored and measuring points analyzed. The data are stored in the 256 MB internal memory and also on a SD card or USB stick. |
| | Technical Information TI00133R Operating Instructions BA00247R |
| Cerabar M | The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value. |
| | Technical Information TI00426P and TI00436P Operating Instructions BA00200P and BA00382P |

| Accessories | Description |
|-------------|--|
| Cerabar S | The pressure transmitter for measuring the absolute and gauge pressure of gases, steam and liquids. It can be used to read in the operating pressure value. |
| | Technical Information TI00383POperating Instructions BA00271P |
| iTEMP | The temperature transmitters can be used in all applications and are suitable for the measurement of gases, steam and liquids. They can be used to read in the medium temperature. |
| | "Fields of Activity" document FA00006T |

Supplementary documentation



For an overview of the scope of the associated Technical Documentation, refer to the following:

- *W@M Device Viewer* (www.endress.com/deviceviewer): Enter the serial number from
- Endress+Hauser Operations App: Enter the serial number from the nameplate or scan the 2D matrix code (QR code) on the nameplate

Standard documentation **Brief Operating Instructions**

Brief Operating Instructions for the sensor

| Measuring device | Documentation code |
|-------------------|--------------------|
| Proline Promass H | KA01283D |

Brief Operating Instructions for transmitter

| | Documentation code | | | | | | |
|-----------------------|--------------------|------------------------|-------------|-------------|--------------|-------------|----------|
| Measuring device | HART | FOUNDATION Fieldbus | PROFIBUS PA | PROFIBUS DP | Modbus RS485 | EtherNet/IP | PROFINET |
| Proline 500 – digital | KA01315D | KA01233D | KA01392D | KA01390D | KA01319D | KA01346D | KA01351D |
| Proline 500 | KA01314D | KA01291D | KA01391D | KA01389D | KA01318D | KA01347D | KA01350D |

Operating Instructions

| Measuring device | Documentation code | | | | | | |
|------------------|--------------------|------------------------|-------------|-------------|--------------|-------------|----------|
| | HART | FOUNDATION Fieldbus | PROFIBUS PA | PROFIBUS DP | Modbus RS485 | EtherNet/IP | PROFINET |
| Promass H 500 | BA01530D | BA01563D | BA01552D | BA01874D | BA01541D | BA01751D | BA01762D |

Description of Device Parameters

| | Documentation code | | | | | | |
|------------------|--------------------|------------------------|-------------|-------------|--------------|-------------|----------|
| Measuring device | HART | FOUNDATION Fieldbus | PROFIBUS PA | PROFIBUS DP | Modbus RS485 | EtherNet/IP | PROFINET |
| Promass 500 | GP01060D | GP01096D | GP01061D | GP01137D | GP01062D | GP01120D | GP01121D |

Device-dependent additional documentation

Safety instructions

Safety instructions for electrical equipment for hazardous areas.

| Contents | Documentation code |
|------------------|--------------------|
| | Measuring device |
| ATEX/IECEx Ex i | XA01473D |
| ATEX/IECEx Ex ec | XA01474D |
| cCSAus IS | XA01475D |
| cCSAus Ex i | XA01509D |
| cCSAus Ex nA | XA01510D |
| INMETRO Ex i | XA01476D |
| INMETRO Ex ec | XA01477D |
| NEPSI Ex i | XA01478D |
| NEPSI Ex nA | XA01479D |

Special Documentation

| Contents | Documentation code |
|---|--------------------|
| Information on the Pressure Equipment Directive | SD01614D |
| Functional Safety Manual | SD01729D |
| Radio approvals for WLAN interface for A309/A310 display module | SD01793D |
| OPC-UA Server 1) | SD02040D |

1) This Special Documentation is only available for device versions with a HART output.

| Contents | Documentation code | | | | | | |
|---------------------------|--------------------|------------------------|-------------|-------------|--------------|----------|-------------|
| | HART | FOUNDATION Fieldbus | PROFIBUS PA | PROFIBUS DP | Modbus RS485 | PROFINET | EtherNet/IP |
| Web server | SD01666D | SD01669D | SD01668D | SD02232D | SD01667D | SD01971D | SD01970D |
| Heartbeat Technology | SD01643D | SD01608D | SD01705D | SD02203D | SD01704D | SD01989D | SD01983D |
| Concentration measurement | SD01645D | SD01709D | SD01711D | SD02213D | SD01710D | SD02007D | SD02006D |

Installation Instructions

| Contents | Comment |
|---|---|
| Installation instructions for spare part sets and accessories | Documentation code: specified for each individual accessory . |

Registered trademarks

HART®

Registered trademark of the FieldComm Group, Austin, Texas, USA $\,$

PROFIBUS®

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany

FOUNDATION™ Fieldbus

Registration-pending trademark of the FieldComm Group, Austin, Texas, USA

102

Modbus[®]

Registered trademark of SCHNEIDER AUTOMATION, INC.

EtherNet/IPTM

Trademark of ODVA, Inc.

PROFINET®

 $Registered\ trademark\ of\ the\ PROFIBUS\ User\ Organization,\ Karlsruhe,\ Germany$



